

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019955.D
 Acq On : 08 Jan 2021 18:22
 Operator : SY/MD
 Sample : M1064-04DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	80	rVB	158914	159101	8.89%	1.074%
2	1.569	143	149	163	rVB	165786	186734	10.44%	1.261%
3	2.110	309	317	344	rVB	303650	485049	27.11%	3.276%
4	2.438	417	419	421	rBV2	906	470	0.03%	0.003%
5	2.486	430	434	435	rBV4	790	530	0.03%	0.004%
6	2.518	435	444	447	rVV6	2712	4023	0.22%	0.027%
7	2.592	465	467	469	rBV2	610	329	0.02%	0.002%
8	2.714	502	505	507	rBV4	1152	719	0.04%	0.005%
9	2.820	534	538	542	rBV2	1036	914	0.05%	0.006%
10	2.917	564	568	572	rBV4	713	660	0.04%	0.004%
11	2.974	584	586	589	rBV4	658	489	0.03%	0.003%
12	3.180	646	650	652	rBV	770	570	0.03%	0.004%
13	3.315	689	692	696	rBV3	706	366	0.02%	0.002%
14	3.396	714	717	721	rBV3	1052	651	0.04%	0.004%
15	3.515	752	754	756	rBV3	714	419	0.02%	0.003%
16	3.608	780	783	786	rBV3	850	442	0.02%	0.003%
17	3.627	786	789	791	rVV3	585	361	0.02%	0.002%
18	3.650	792	796	798	rVB3	856	573	0.03%	0.004%
19	3.692	804	809	811	rBV4	955	937	0.05%	0.006%
20	3.727	816	820	822	rVB2	631	485	0.03%	0.003%
21	3.772	830	834	840	rVB6	1238	1324	0.07%	0.009%
22	3.804	840	844	846	rBV4	953	525	0.03%	0.004%
23	3.817	846	848	851	rVB3	696	373	0.02%	0.003%
24	3.836	851	854	856	rBV4	1070	702	0.04%	0.005%
25	3.888	859	870	905	rBV	163919	474664	26.53%	3.205%
26	4.354	1001	1015	1043	rVB	264561	645523	36.08%	4.359%
27	4.888	1178	1181	1185	rBV2	1259	1069	0.06%	0.007%
28	4.955	1199	1202	1203	rBV2	615	411	0.02%	0.003%
29	5.052	1212	1232	1257	rBV2	584154	1534572	85.78%	10.363%
30	5.479	1358	1365	1366	rBV4	1946	1894	0.11%	0.013%
31	5.518	1375	1377	1380	rBV4	800	535	0.03%	0.004%
32	5.621	1397	1409	1440	rBV	577000	1158112	64.74%	7.821%
33	5.916	1486	1501	1532	rBV4	77492	190817	10.67%	1.289%
34	6.074	1538	1550	1570	rBV	372593	744703	41.63%	5.029%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019955.D
 Acq On : 08 Jan 2021 18:22
 Operator : SY/MD
 Sample : M1064-04DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	6.537	1692	1694	1696	rBV3	793	455	0.03%	0.003%
36	6.566	1701	1703	1705	rBV2	788	384	0.02%	0.003%
37	6.633	1716	1724	1726	rBV7	1794	2377	0.13%	0.016%
38	6.772	1764	1767	1768	rBV2	645	384	0.02%	0.003%
39	6.875	1797	1799	1801	rVB3	933	422	0.02%	0.003%
40	6.907	1806	1809	1813	rVB3	747	485	0.03%	0.003%
41	6.936	1816	1818	1822	rBV5	648	469	0.03%	0.003%
42	6.990	1824	1835	1858	rBV	175406	330950	18.50%	2.235%
43	7.277	1922	1924	1926	rBV2	954	554	0.03%	0.004%
44	7.322	1926	1938	1964	rVV	611797	1073397	60.00%	7.249%
45	7.547	2006	2008	2014	rBV5	839	787	0.04%	0.005%
46	7.627	2023	2033	2055	rBV	123615	216500	12.10%	1.462%
47	7.910	2114	2121	2123	rVB8	963	886	0.05%	0.006%
48	7.923	2123	2125	2128	rBV3	569	385	0.02%	0.003%
49	7.981	2128	2143	2162	rBV	1073409	1788925	100.00%	12.081%
50	8.093	2168	2178	2218	rBV2	480210	945348	52.84%	6.384%
51	8.695	2363	2365	2371	rVB3	1323	905	0.05%	0.006%
52	8.791	2393	2395	2399	rBV5	648	383	0.02%	0.003%
53	8.858	2404	2416	2439	rBV	888096	1438257	80.40%	9.713%
54	9.248	2534	2537	2540	rVB3	1871	1399	0.08%	0.009%
55	9.267	2540	2543	2546	rBV4	1352	880	0.05%	0.006%
56	9.286	2546	2549	2550	rBV4	979	481	0.03%	0.003%
57	9.341	2565	2566	2569	rBV3	661	414	0.02%	0.003%
58	9.447	2596	2599	2601	rBV4	672	444	0.02%	0.003%
59	9.502	2614	2616	2618	rBV2	1005	500	0.03%	0.003%
60	9.547	2629	2630	2632	rBV2	772	384	0.02%	0.003%
61	9.630	2653	2656	2659	rBV4	1092	662	0.04%	0.004%
62	9.649	2659	2662	2664	rBV3	629	410	0.02%	0.003%
63	9.752	2690	2694	2695	rBV2	697	461	0.03%	0.003%
64	9.852	2722	2725	2728	rBV4	684	523	0.03%	0.004%
65	10.019	2775	2777	2781	rVB3	978	601	0.03%	0.004%
66	10.064	2787	2791	2792	rBV2	740	406	0.02%	0.003%
67	10.112	2803	2806	2807	rBV3	929	525	0.03%	0.004%
68	10.154	2817	2819	2823	rBV3	874	573	0.03%	0.004%
69	10.222	2828	2840	2862	rBV	517963	821070	45.90%	5.545%
70	10.492	2920	2924	2928	rBV5	1077	1079	0.06%	0.007%
71	10.540	2938	2939	2941	rBV	846	447	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019955.D
 Acq On : 08 Jan 2021 18:22
 Operator : SY/MD
 Sample : M1064-04DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.704	2983	2990	2994	rBV7	1482	1827	0.10%	0.012%
73	10.727	2994	2997	2999	rVV4	1071	687	0.04%	0.005%
74	10.743	2999	3002	3004	rBV3	612	342	0.02%	0.002%
75	10.781	3012	3014	3016	rBV2	835	419	0.02%	0.003%
76	10.817	3023	3025	3029	rVB2	1239	806	0.05%	0.005%
77	10.849	3031	3035	3040	rBV6	1346	1493	0.08%	0.010%
78	10.990	3075	3079	3082	rBV5	1063	1011	0.06%	0.007%
79	11.180	3136	3138	3141	rBV5	1045	754	0.04%	0.005%
80	11.215	3146	3149	3150	rBV3	1114	519	0.03%	0.004%
81	11.257	3150	3162	3183	rBV	884774	1375738	76.90%	9.290%
82	11.630	3266	3278	3297	rBV	741355	1179677	65.94%	7.966%
83	11.881	3353	3356	3357	rBV3	1313	683	0.04%	0.005%
84	11.916	3364	3367	3369	rBV3	853	571	0.03%	0.004%
85	12.029	3400	3402	3408	rVB5	990	833	0.05%	0.006%
86	12.199	3453	3455	3458	rVB3	1101	579	0.03%	0.004%
87	12.215	3458	3460	3462	rBV2	812	480	0.03%	0.003%
88	12.427	3523	3526	3529	rBV4	1092	707	0.04%	0.005%
89	12.633	3587	3590	3593	rVB3	1078	517	0.03%	0.003%
90	12.717	3614	3616	3618	rBV2	943	491	0.03%	0.003%
91	12.955	3688	3690	3692	rBV2	630	345	0.02%	0.002%
92	13.190	3760	3763	3767	rBV2	1131	925	0.05%	0.006%
93	13.373	3818	3820	3823	rBV2	561	360	0.02%	0.002%
94	13.434	3837	3839	3841	rBV2	800	388	0.02%	0.003%
95	13.862	3970	3972	3973	rBV	793	379	0.02%	0.003%
96	13.993	4010	4013	4016	rBV3	1152	743	0.04%	0.005%
97	14.042	4025	4028	4029	rBV2	1101	613	0.03%	0.004%
98	14.505	4167	4172	4174	rBV5	1637	1362	0.08%	0.009%
99	14.546	4183	4185	4187	rBV2	1036	517	0.03%	0.003%
100	14.620	4200	4208	4210	rBV4	1648	1967	0.11%	0.013%


Sum of corrected areas: 14808291

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019955.D
Acq On : 08 Jan 2021 18:22
Operator : SY/MD
Sample : M1064-04DL 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

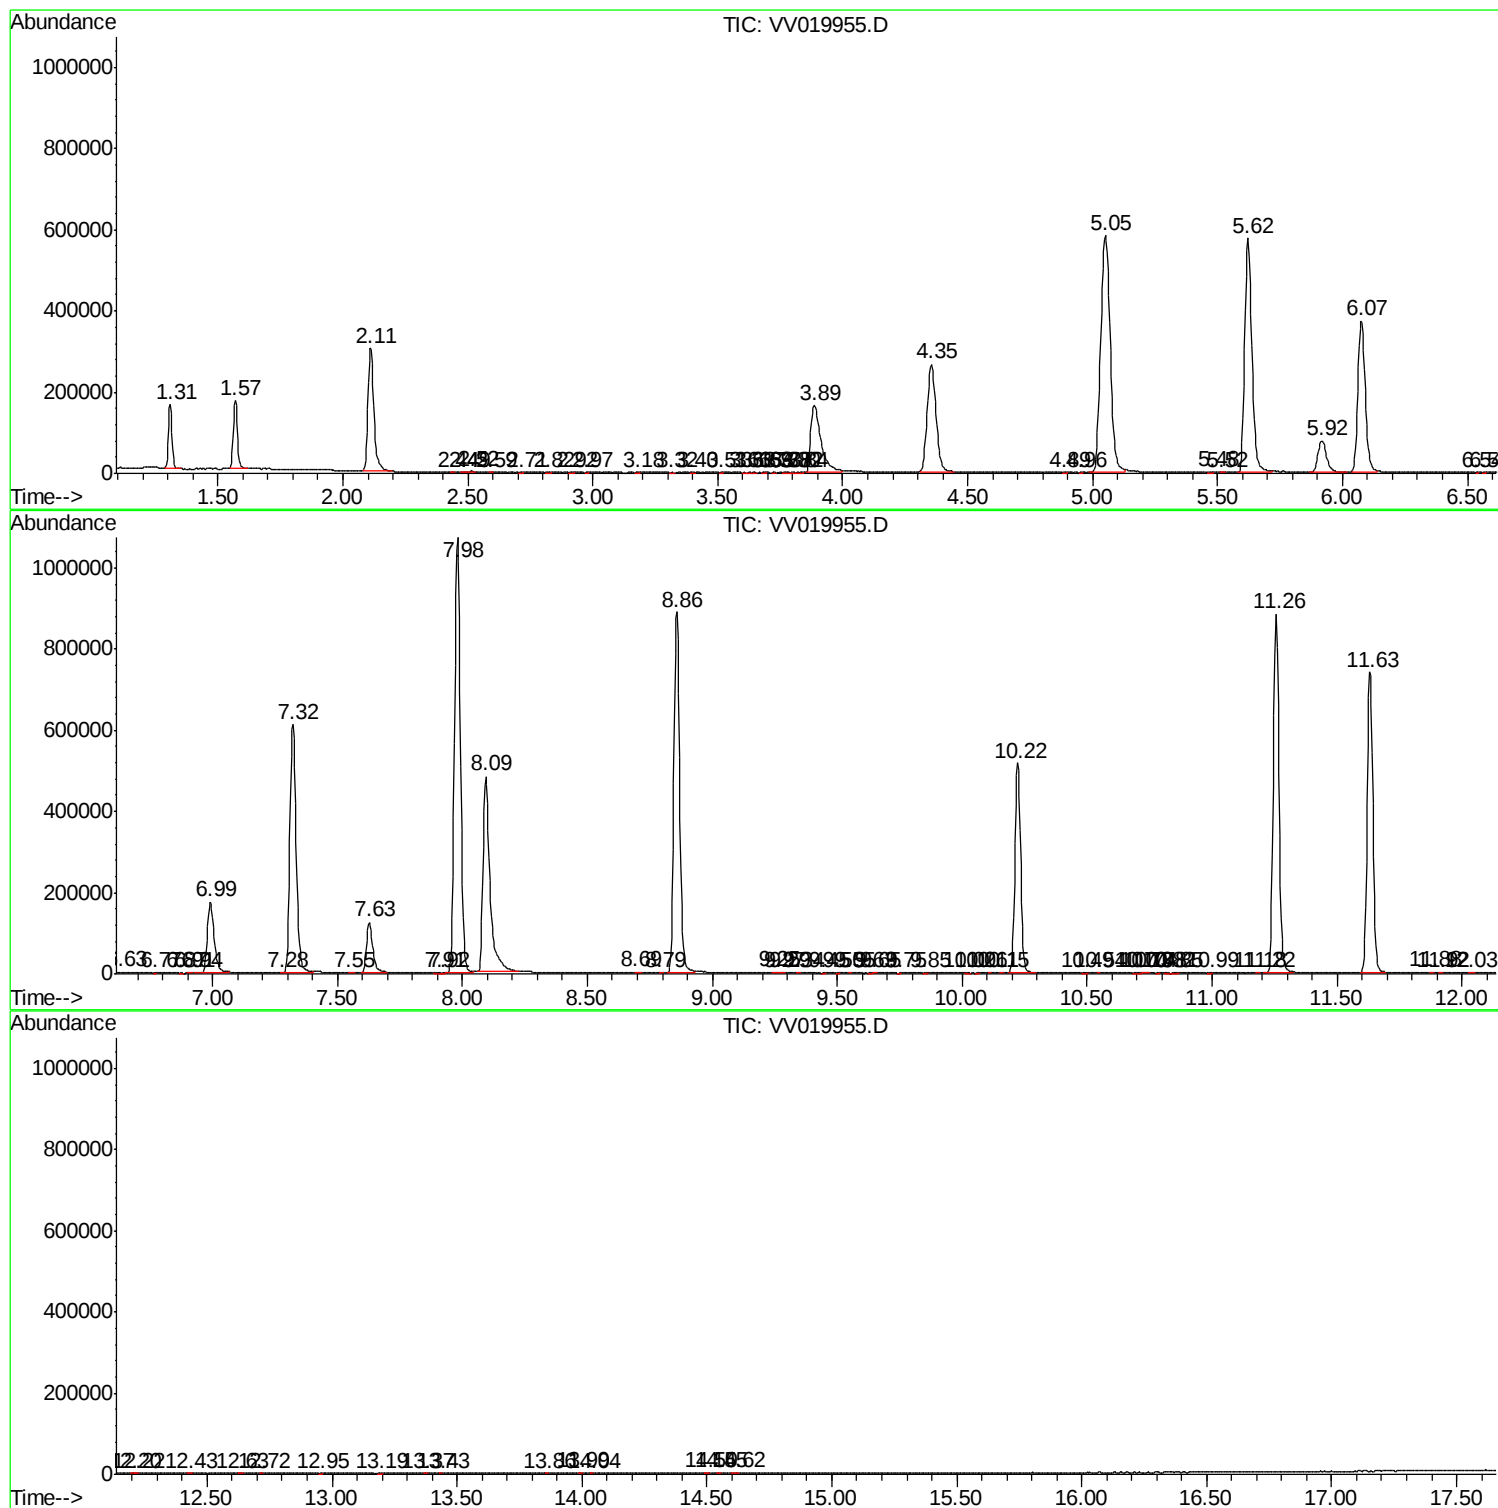

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019955.D
Acq On : 08 Jan 2021 18:22
Operator : SY/MD
Sample : M1064-04DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV010821\
Data File : VV019955.D
Acq On : 08 Jan 2021 18:22
Operator : SY/MD
Sample : M1064-04DL 500X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4X5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc