

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019956.D
 Acq On : 08 Jan 2021 18:45
 Operator : SY/MD
 Sample : VIBLK79
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	80	rVB	241366	237824	12.59%	1.731%
2	1.570	142	149	161	rVB	228326	253664	13.43%	1.846%
3	2.110	308	317	340	rVB	422596	646567	34.24%	4.706%
4	2.441	418	420	423	rBV2	842	535	0.03%	0.004%
5	2.492	434	436	437	rBV	1170	475	0.03%	0.003%
6	2.698	497	500	503	rVB3	841	486	0.03%	0.004%
7	2.724	503	508	513	rBV6	1140	1672	0.09%	0.012%
8	2.824	536	539	540	rBV3	1071	565	0.03%	0.004%
9	2.881	554	557	560	rBV4	742	493	0.03%	0.004%
10	2.901	560	563	565	rVV	795	323	0.02%	0.002%
11	3.010	594	597	600	rBV3	733	594	0.03%	0.004%
12	3.090	618	622	625	rBV5	696	653	0.03%	0.005%
13	3.180	645	650	654	rBV4	1385	1461	0.08%	0.011%
14	3.264	673	676	678	rBV4	1222	823	0.04%	0.006%
15	3.293	683	685	688	rBV3	1077	397	0.02%	0.003%
16	3.335	695	698	701	rVB3	1147	719	0.04%	0.005%
17	3.393	711	716	717	rBV3	960	811	0.04%	0.006%
18	3.444	729	732	733	rBV	623	367	0.02%	0.003%
19	3.489	742	746	749	rVB5	1102	926	0.05%	0.007%
20	3.521	749	756	760	rBV6	1588	1546	0.08%	0.011%
21	3.557	764	767	769	rBV3	494	327	0.02%	0.002%
22	3.589	772	777	779	rBV3	1312	1069	0.06%	0.008%
23	3.631	787	790	793	rBV3	646	425	0.02%	0.003%
24	3.885	859	869	898	rBV	160855	450213	23.84%	3.277%
25	4.354	1001	1015	1043	rVB	310135	755149	39.99%	5.496%
26	4.749	1134	1138	1139	rBV4	706	457	0.02%	0.003%
27	4.759	1139	1141	1144	rBV3	842	634	0.03%	0.005%
28	4.794	1149	1152	1154	rBV4	1098	669	0.04%	0.005%
29	4.840	1162	1166	1168	rBV5	1158	867	0.05%	0.006%
30	4.952	1195	1201	1204	rBV6	1213	1401	0.07%	0.010%
31	5.052	1215	1232	1264	rBV2	731310	1888444	100.00%	13.744%
32	5.409	1339	1343	1344	rBV3	1603	1110	0.06%	0.008%
33	5.441	1350	1353	1355	rBV4	656	411	0.02%	0.003%
34	5.457	1356	1358	1360	rBV2	743	360	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019956.D
 Acq On : 08 Jan 2021 18:45
 Operator : SY/MD
 Sample : VIBLK79
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	5.470	1360	1362	1365	rVV2	1193	694	0.04%	0.005%
36	5.537	1378	1383	1386	rBV5	1043	1055	0.06%	0.008%
37	5.576	1393	1395	1396	rBV2	652	313	0.02%	0.002%
38	5.621	1397	1409	1436	rVV	464114	946673	50.13%	6.890%
39	5.910	1490	1499	1517	rVB4	39403	79933	4.23%	0.582%
40	6.074	1533	1550	1580	rBV	442219	901115	47.72%	6.558%
41	6.556	1697	1700	1705	rBV6	1397	1410	0.07%	0.010%
42	6.618	1716	1719	1720	rBV2	609	347	0.02%	0.003%
43	6.855	1791	1793	1795	rBV2	538	307	0.02%	0.002%
44	6.875	1797	1799	1805	rVB5	1179	1023	0.05%	0.007%
45	6.991	1823	1835	1858	rBV	223990	413476	21.90%	3.009%
46	7.322	1926	1938	1960	rBV	814537	1397939	74.03%	10.174%
47	7.627	2022	2033	2055	rBV	154431	274601	14.54%	1.999%
48	7.910	2119	2121	2122	rBV2	1254	490	0.03%	0.004%
49	7.981	2136	2143	2153	rVB6	7778	12649	0.67%	0.092%
50	8.055	2162	2166	2168	rBV2	1042	924	0.05%	0.007%
51	8.093	2168	2178	2222	rVV2	468179	955522	50.60%	6.954%
52	8.727	2373	2375	2382	rBV6	925	1054	0.06%	0.008%
53	8.859	2404	2416	2447	rBV	720543	1177975	62.38%	8.573%
54	9.293	2548	2551	2553	rBV3	560	360	0.02%	0.003%
55	9.344	2564	2567	2572	rVB3	999	961	0.05%	0.007%
56	9.431	2591	2594	2596	rBV4	1197	873	0.05%	0.006%
57	9.473	2603	2607	2612	rBV7	1368	1197	0.06%	0.009%
58	9.543	2622	2629	2631	rBV5	1356	1410	0.07%	0.010%
59	9.855	2723	2726	2730	rVB5	1049	821	0.04%	0.006%
60	9.881	2730	2734	2738	rBV5	794	717	0.04%	0.005%
61	9.920	2743	2746	2749	rBV3	1167	825	0.04%	0.006%
62	9.994	2765	2769	2772	rBV6	1308	1159	0.06%	0.008%
63	10.068	2788	2792	2794	rBV3	515	419	0.02%	0.003%
64	10.135	2811	2813	2816	rBV3	839	588	0.03%	0.004%
65	10.222	2828	2840	2865	rBV	535651	836024	44.27%	6.085%
66	10.376	2882	2888	2892	rBV7	1060	1417	0.08%	0.010%
67	10.460	2912	2914	2918	rBV3	976	609	0.03%	0.004%
68	10.482	2918	2921	2926	rVB5	1152	821	0.04%	0.006%
69	10.553	2939	2943	2949	rVB6	1678	1901	0.10%	0.014%
70	10.582	2950	2952	2953	rBV2	772	314	0.02%	0.002%
71	10.730	2994	2998	2999	rBV	579	431	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV010821\
 Data File : VV019956.D
 Acq On : 08 Jan 2021 18:45
 Operator : SY/MD
 Sample : VIBLK79
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

72	10.765	3007	3009	3010	rBV	767	305	0.02%	0.002%
73	10.817	3023	3025	3027	rBV3	715	318	0.02%	0.002%
74	10.871	3039	3042	3044	rBV3	843	497	0.03%	0.004%
75	10.929	3054	3060	3062	rBV4	1138	1079	0.06%	0.008%
76	10.974	3072	3074	3076	rBV2	653	327	0.02%	0.002%
77	11.032	3090	3092	3094	rBV2	753	324	0.02%	0.002%
78	11.087	3105	3109	3111	rBV3	538	407	0.02%	0.003%
79	11.106	3113	3115	3118	rVV2	842	551	0.03%	0.004%
80	11.122	3118	3120	3122	rVB3	1070	449	0.02%	0.003%
81	11.138	3122	3125	3127	rBV2	732	412	0.02%	0.003%
82	11.199	3142	3144	3146	rVB2	1260	590	0.03%	0.004%
83	11.257	3150	3162	3180	rBV	713243	1118251	59.22%	8.139%
84	11.412	3207	3210	3213	rBV2	1426	771	0.04%	0.006%
85	11.518	3241	3243	3246	rBV3	801	324	0.02%	0.002%
86	11.630	3266	3278	3296	rBV	842390	1333617	70.62%	9.706%
87	11.846	3341	3345	3347	rBV3	1390	1034	0.05%	0.008%
88	12.334	3496	3497	3500	rBV3	932	436	0.02%	0.003%
89	12.424	3522	3525	3527	rBV2	1043	552	0.03%	0.004%
90	12.479	3540	3542	3546	rVB5	1300	701	0.04%	0.005%
91	12.617	3581	3585	3587	rBV4	873	620	0.03%	0.005%
92	12.804	3640	3643	3648	rBV6	1217	1115	0.06%	0.008%
93	12.887	3667	3669	3674	rBV3	770	557	0.03%	0.004%
94	13.106	3732	3737	3741	rBV6	1254	1332	0.07%	0.010%
95	13.231	3773	3776	3778	rVB2	903	477	0.03%	0.003%
96	13.752	3934	3938	3941	rBV2	1415	869	0.05%	0.006%
97	13.768	3941	3943	3944	rBV2	810	417	0.02%	0.003%
98	14.309	4108	4111	4115	rBV4	1508	1386	0.07%	0.010%
99	14.534	4179	4181	4185	rBV4	1009	545	0.03%	0.004%
100	15.453	4462	4467	4468	rBV4	1366	1089	0.06%	0.008%


Sum of corrected areas: 13740136

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV010821\
Data File : VV019956.D
Acq On : 08 Jan 2021 18:45
Operator : SY/MD
Sample : VIBLK79
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

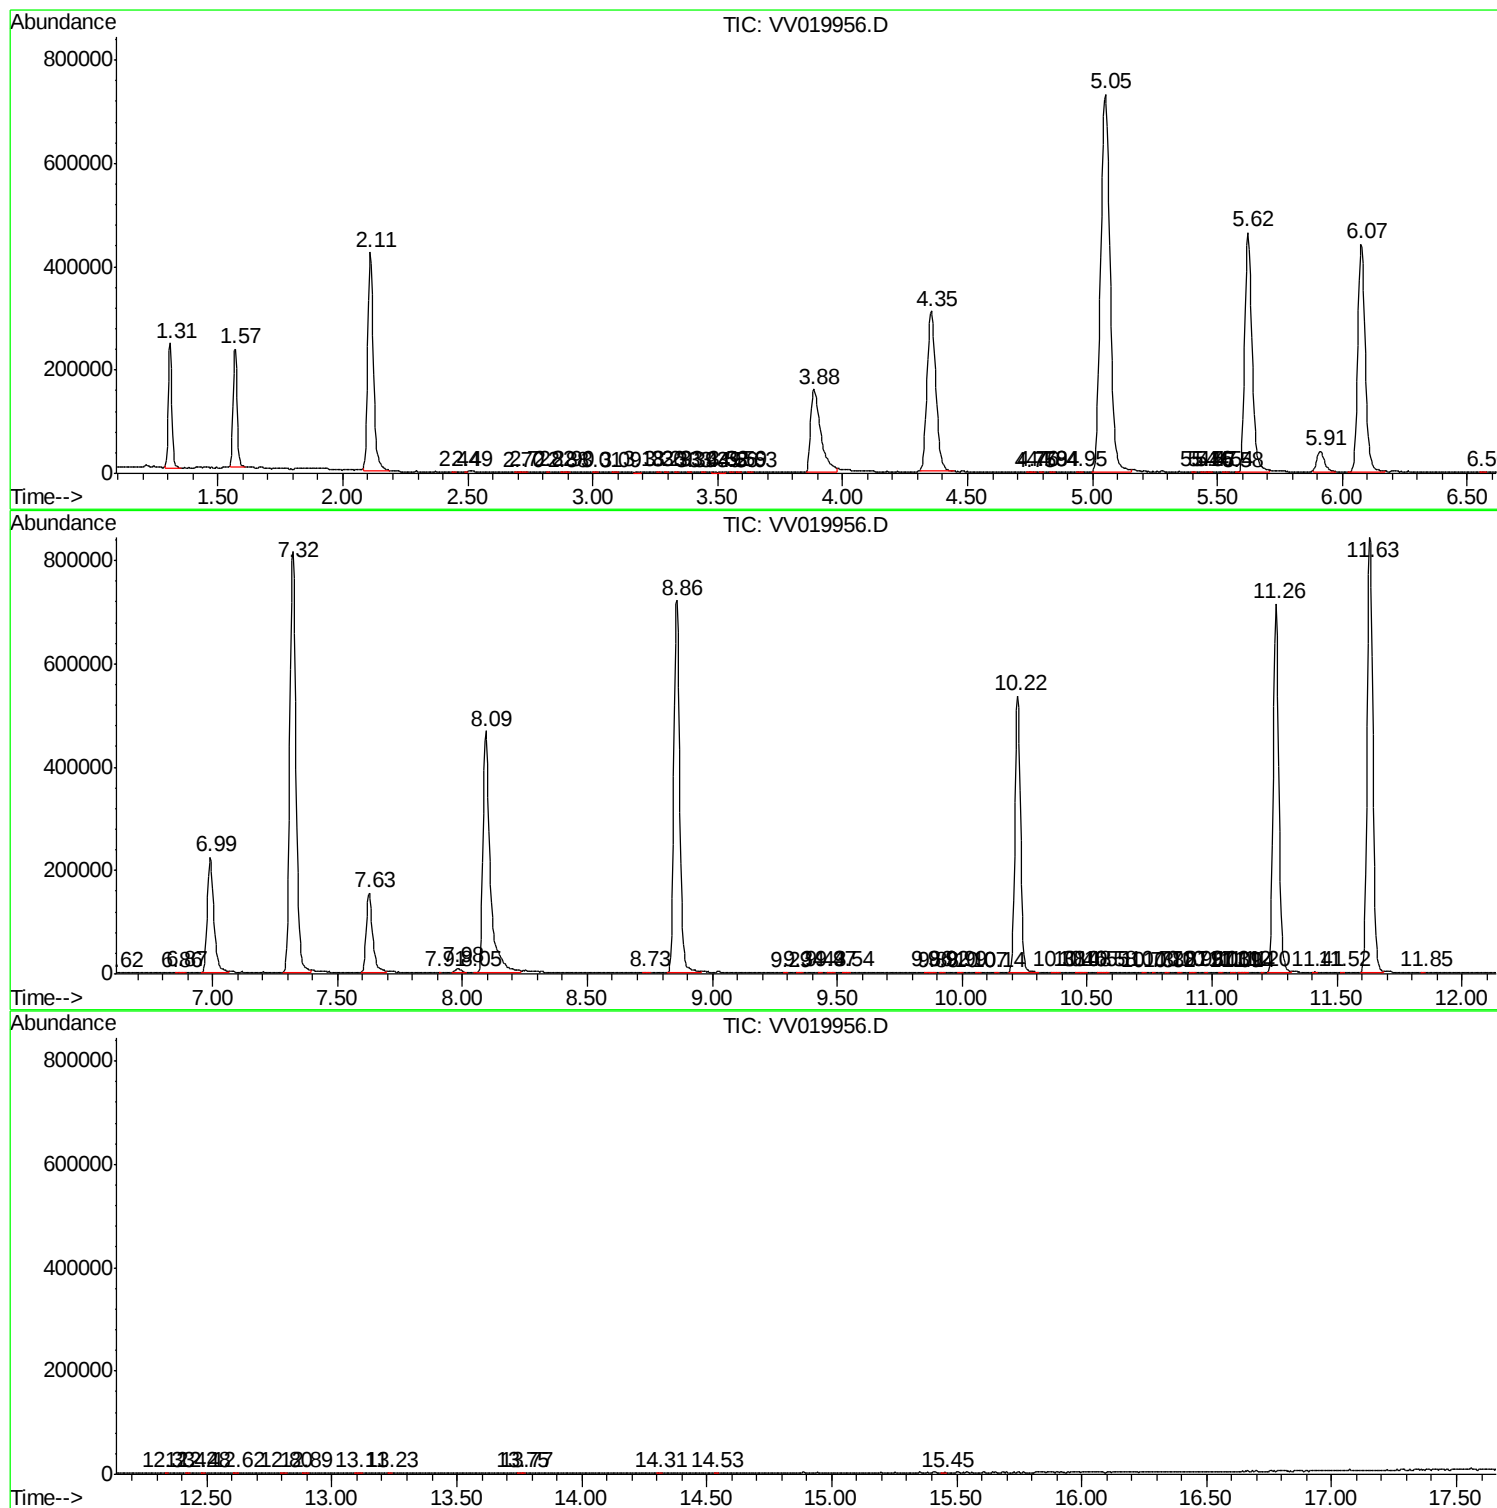

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019956.D
Acq On : 08 Jan 2021 18:45
Operator : SY/MD
Sample : VIBLK79
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV010821\
Data File : VV019956.D
Acq On : 08 Jan 2021 18:45
Operator : SY/MD
Sample : VIBLK79
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc