


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV010821\
 Data File : VV019936.D
 Acq On : 08 Jan 2021 08:49
 Operator : SY/MD
 Sample : BFB77
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB77

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 08 22:51:06 2021

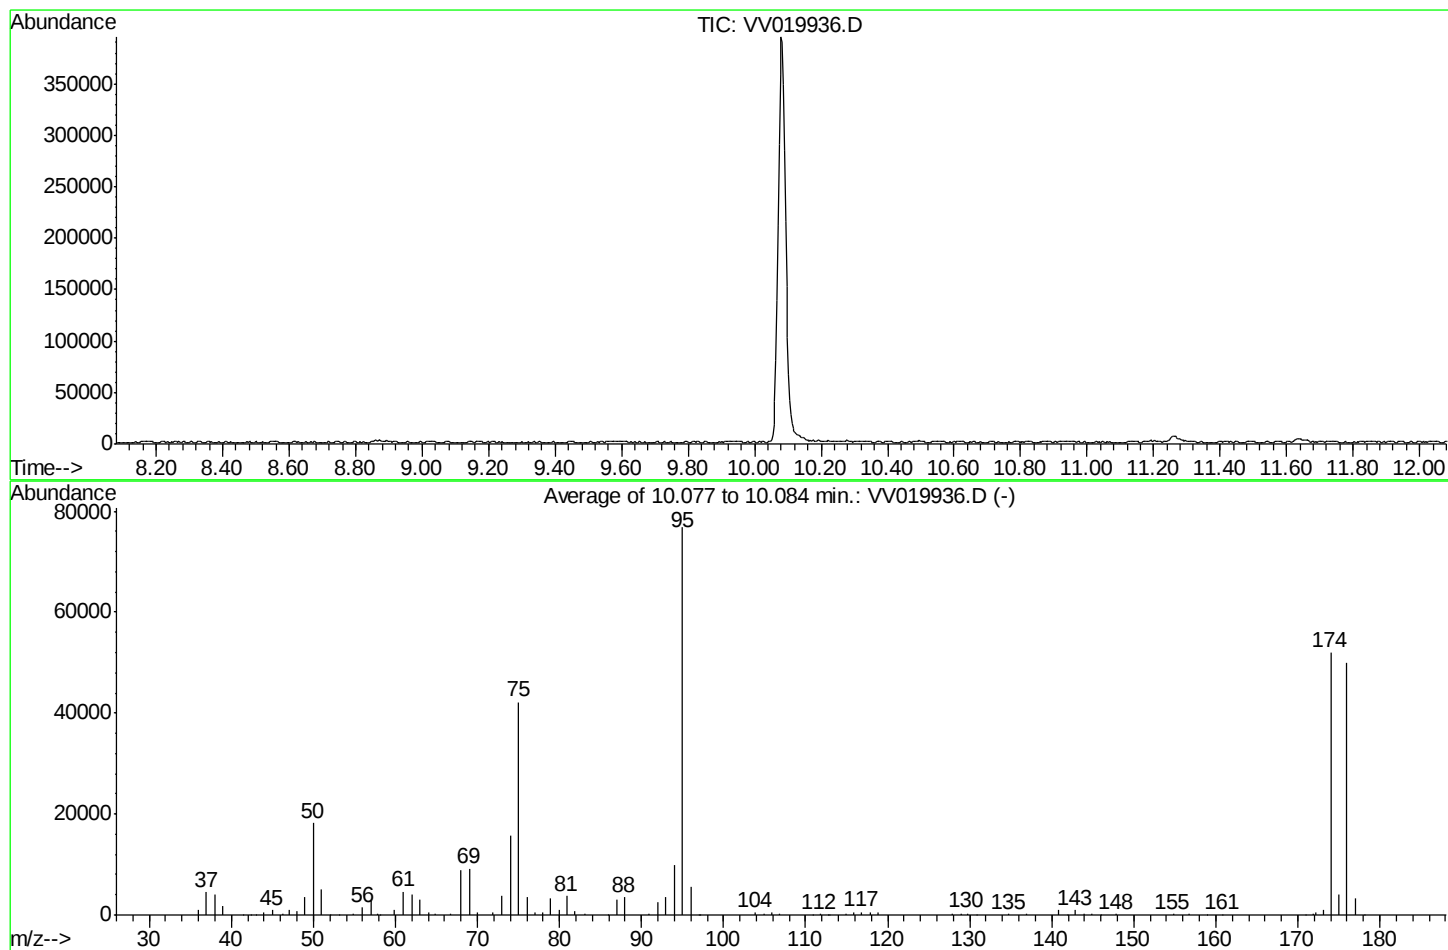

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	18157	PASS
75	95	30	80	54.9	42170	PASS
95	95	100	100	100.0	76826	PASS
96	95	5	9	7.3	5643	PASS
173	174	0.00	2	1.8	936	PASS
174	95	50	120	67.6	51925	PASS
175	174	5	9	8.1	4180	PASS
176	174	95	101	96.5	50082	PASS
177	176	5	9	6.4	3206	PASS

Scan 2785 (10.045 min): VV019936.D
BFB77

m/z	Abundance
35.20	126.0
36.30	120.0
36.90	107.0
37.90	132.0
40.00	376.0
41.80	118.0
43.10	117.0
43.90	544.0
45.50	124.0
47.40	110.0
49.80	139.0
50.80	123.0
52.20	126.0
65.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	950.0
37.00	4315.0
38.00	3958.0
39.00	1867.0
40.00	253.0
41.50	115.0
42.30	108.0
43.10	159.0
44.00	1094.0
45.00	805.0
46.20	207.0
47.00	956.0
48.00	524.0
49.00	3504.0
50.00	17656.0
51.00	4953.0
52.00	274.0
54.90	353.0
56.00	1484.0
57.00	2480.0
57.90	132.0
58.20	111.0
59.90	911.0
61.00	4359.0
62.00	3919.0
63.00	3021.0
64.00	435.0
64.90	401.0
66.80	287.0
68.00	8416.0
69.00	8618.0
70.00	571.0
71.90	434.0
73.00	3780.0
74.00	14934.0
75.00	39696.0
76.00	3544.0
77.00	518.0
77.80	354.0
78.90	3234.0
79.90	1006.0
80.90	3460.0
81.90	812.0
83.00	152.0
85.90	131.0
86.90	2845.0
87.90	3091.0
90.80	296.0
92.00	2343.0
93.00	3597.0
94.00	9358.0
95.00	72648.0
96.00	5551.0
96.90	120.0
103.90	404.0
104.90	205.0
105.80	393.0
106.80	141.0
110.90	117.0
111.80	182.0
112.70	137.0
114.90	157.0
115.80	395.0
116.90	506.0
118.00	402.0
118.90	505.0
127.80	258.0
129.00	111.0
129.70	315.0
130.90	120.0
134.80	225.0
136.90	192.0
140.90	855.0
142.90	983.0
143.90	174.0
144.90	152.0
145.90	102.0
147.90	200.0
154.80	174.0
156.90	130.0
158.90	127.0
171.80	405.0
172.20	392.0
173.10	866.0
174.00	47872.0
175.00	3874.0
176.00	45648.0
177.00	3198.0
178.10	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	951.0
37.00	4775.0
38.00	4280.0
39.00	1916.0
40.00	305.0
41.50	101.0
43.00	187.0
44.00	1170.0
45.00	957.0
46.20	224.0
47.00	986.0
48.00	666.0
49.00	3754.0
50.00	18992.0
51.00	5323.0
52.00	257.0
53.10	146.0
54.90	325.0
56.00	1572.0
57.00	2871.0
57.80	139.0
59.90	990.0
61.00	4800.0
62.00	4269.0
63.00	3211.0
64.10	516.0
64.90	417.0
66.70	305.0
68.00	9149.0
69.00	9585.0
69.90	639.0
71.90	431.0
73.00	3994.0
74.00	16155.0
75.00	43568.0
76.00	3692.0
77.00	534.0
77.90	394.0
78.90	3476.0
79.90	1145.0
80.90	3894.0
81.90	928.0
83.00	153.0
85.90	123.0
86.90	3017.0
87.90	3589.0
90.80	300.0
92.00	2578.0
92.90	3772.0
94.00	10120.0
95.00	79632.0
96.00	5845.0
97.00	101.0
103.90	468.0
104.90	213.0
105.80	429.0
106.80	148.0
110.90	140.0
111.80	195.0
112.90	125.0
114.90	182.0
115.80	420.0
116.80	559.0
118.00	417.0
118.90	531.0
127.80	303.0
129.00	132.0
129.70	365.0
130.90	135.0
134.80	222.0
136.90	208.0
140.90	937.0
141.80	130.0
142.90	1000.0
143.90	199.0
145.00	188.0
146.00	133.0
147.90	211.0
154.80	219.0
156.80	150.0
158.90	123.0
160.80	130.0
171.00	162.0
171.80	443.0
172.20	480.0
173.10	1000.0
174.00	53912.0
175.00	4409.0
176.00	52032.0
177.00	3249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.00	840.0
37.00	4750.0
38.00	4238.0
39.00	1796.0
39.90	346.0
43.00	207.0
44.00	1214.0
45.00	969.0
46.20	231.0
47.00	915.0
48.00	743.0
49.00	3696.0
50.00	18240.0
51.00	5261.0
52.00	249.0
53.10	187.0
54.90	350.0
56.00	1391.0
57.00	2938.0
57.90	159.0
59.90	943.0
61.00	4617.0
62.00	4215.0
63.00	3130.0
64.10	508.0
64.90	376.0
66.70	265.0
68.00	9033.0
69.00	9402.0
69.90	705.0
71.90	435.0
73.00	3805.0
74.00	15871.0
75.00	43248.0
76.10	3597.0
77.00	461.0
78.00	440.0
78.90	3522.0
79.90	1116.0
80.90	3803.0
81.90	918.0
83.10	109.0
85.90	118.0
87.00	2948.0
87.90	3637.0
90.90	311.0
91.90	2459.0
93.00	3672.0
94.00	9880.0
95.00	78200.0
96.00	5534.0
97.20	147.0
103.90	492.0
105.00	167.0
105.90	419.0
106.80	142.0
110.90	135.0
111.80	167.0
113.00	144.0
114.90	161.0
115.80	423.0
116.80	530.0
117.90	380.0
118.90	490.0
127.90	343.0
128.80	168.0
129.70	366.0
130.90	129.0
134.80	202.0
136.90	197.0
140.90	923.0
141.90	165.0
142.90	936.0
143.90	174.0
145.00	201.0
146.00	148.0
147.90	208.0
154.80	235.0
156.70	144.0
160.90	151.0
171.00	188.0
172.10	509.0
173.00	942.0
174.00	53992.0
175.00	4257.0
176.00	52568.0
177.00	3172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77