

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010822\
 Data File : VV024310.D
 Acq On : 08 Jan 2022 11:32
 Operator : SY/MD
 Sample : VV0108WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK291

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	93	rVB	56935	57429	16.77%	2.048%
2	1.568	157	164	174	rBV	47458	53305	15.57%	1.901%
3	2.108	321	332	349	rVB	96566	142355	41.57%	5.076%
4	3.912	884	893	916	rBV2	11790	47827	13.97%	1.705%
5	4.342	1012	1027	1052	rVB	62076	161535	47.17%	5.760%
6	5.043	1230	1245	1267	rBV2	137837	342462	100.00%	12.211%
7	5.612	1411	1422	1443	rBV2	112106	227684	66.48%	8.118%
8	6.066	1551	1563	1585	rBV	75122	156098	45.58%	5.566%
9	6.985	1838	1849	1866	rBV	36387	70167	20.49%	2.502%
10	7.313	1939	1951	1969	rBV	165194	288883	84.35%	10.300%
11	7.622	2036	2047	2065	rBV2	22069	41491	12.12%	1.479%
12	8.091	2183	2193	2242	rBV	98063	257253	75.12%	9.173%
13	8.850	2418	2429	2453	rBV	174960	292208	85.33%	10.419%
14	10.214	2843	2853	2868	rBV	49696	81077	23.67%	2.891%
15	11.249	3164	3175	3195	rBV	194123	303636	88.66%	10.827%
16	11.622	3280	3291	3308	rBV	167739	268110	78.29%	9.560%
17	13.268	3794	3803	3811	rVB3	2797	3933	1.15%	0.140%
18	13.512	3869	3879	3887	rBV2	3237	5290	1.54%	0.189%
19	13.747	3944	3952	3961	rVB6	2551	3819	1.12%	0.136%




Sum of corrected areas: 2804562

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010822\
Data File : VV024310.D
Acq On : 08 Jan 2022 11:32
Operator : SY/MD
Sample : VV0108WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK291

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

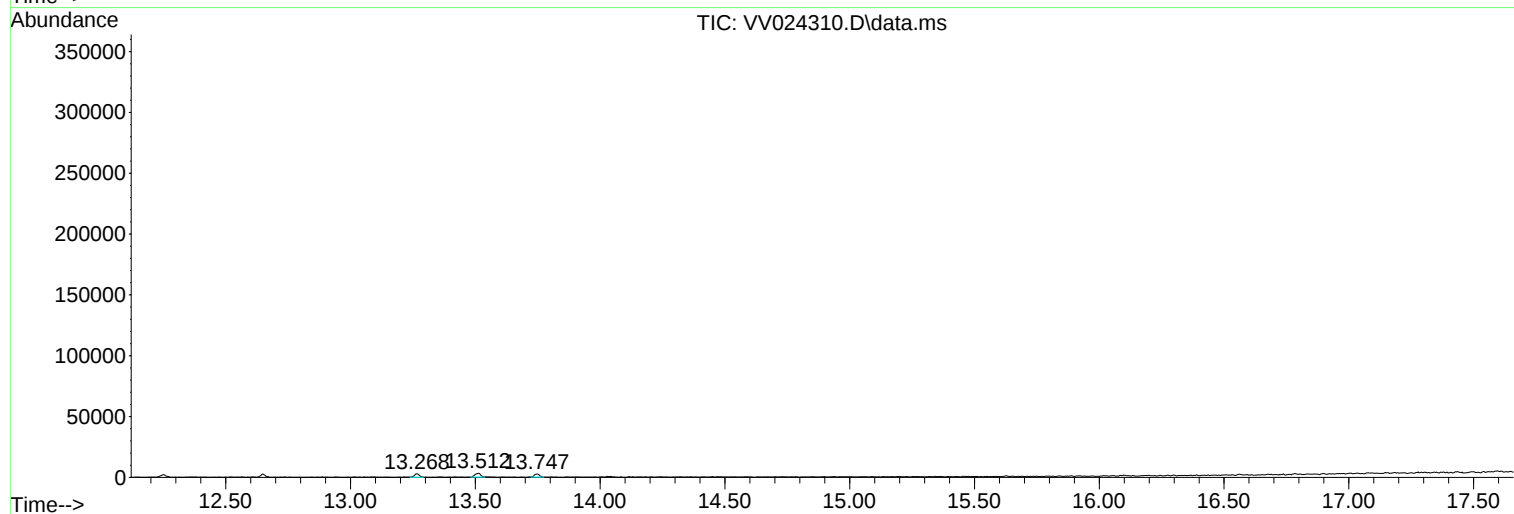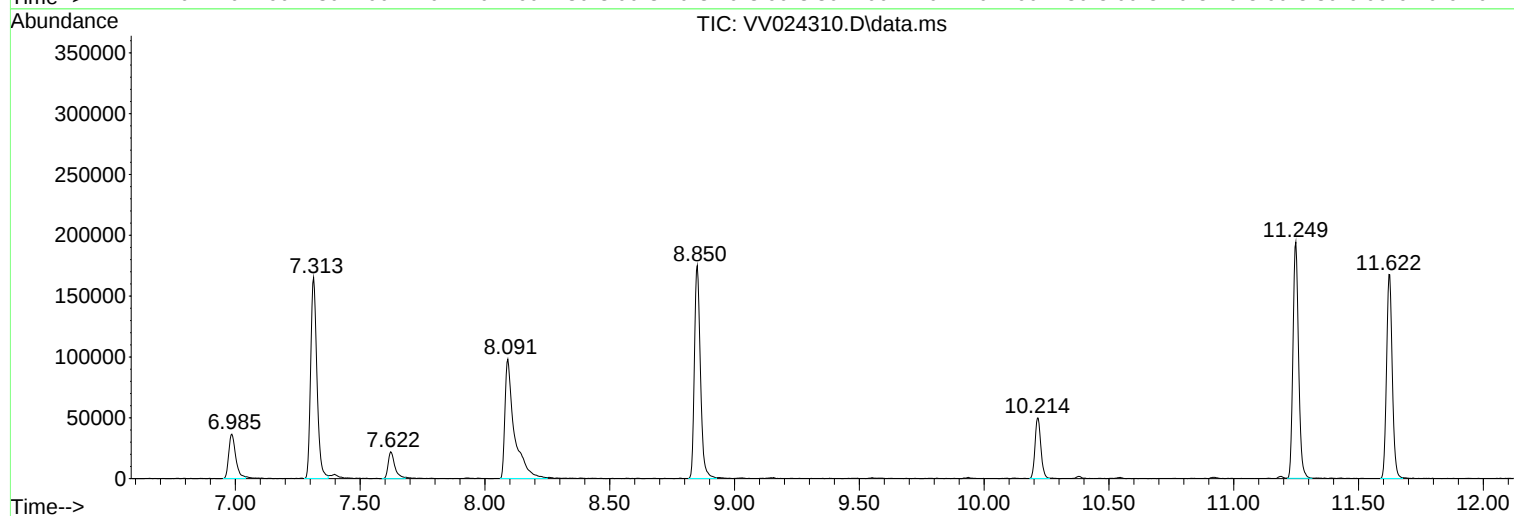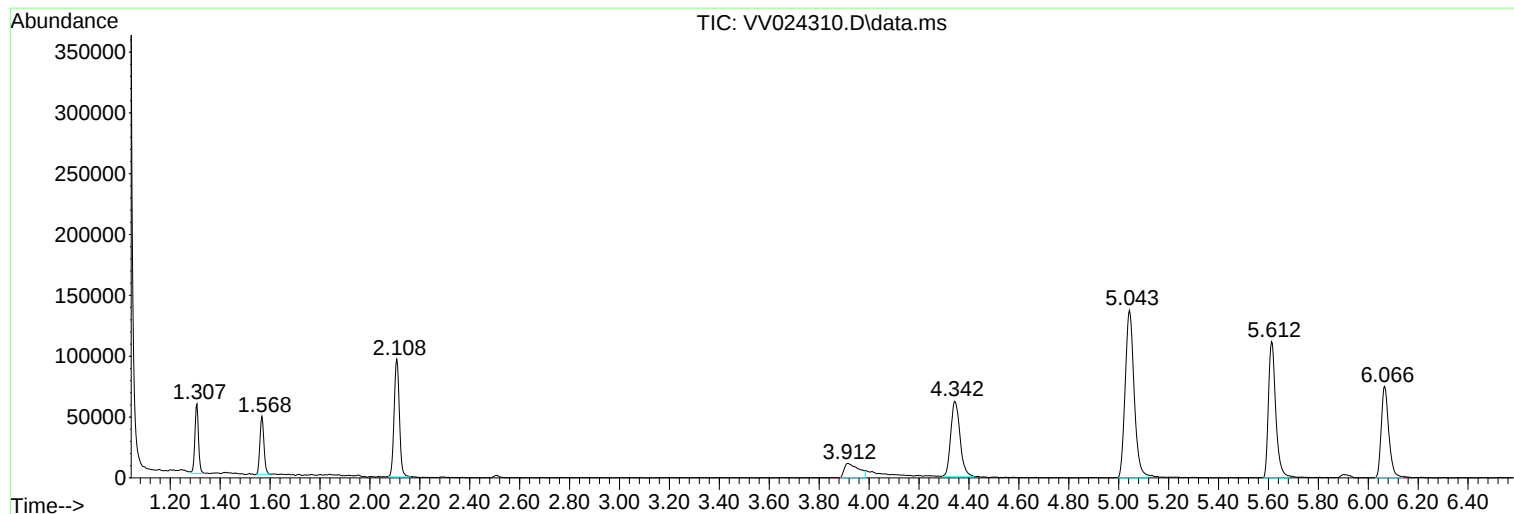

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010822\
Data File : VV024310.D
Acq On : 08 Jan 2022 11:32
Operator : SY/MD
Sample : VV0108WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK291

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010822\
Data File : VV024310.D
Acq On : 08 Jan 2022 11:32
Operator : SY/MD
Sample : VV0108WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK291

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc