
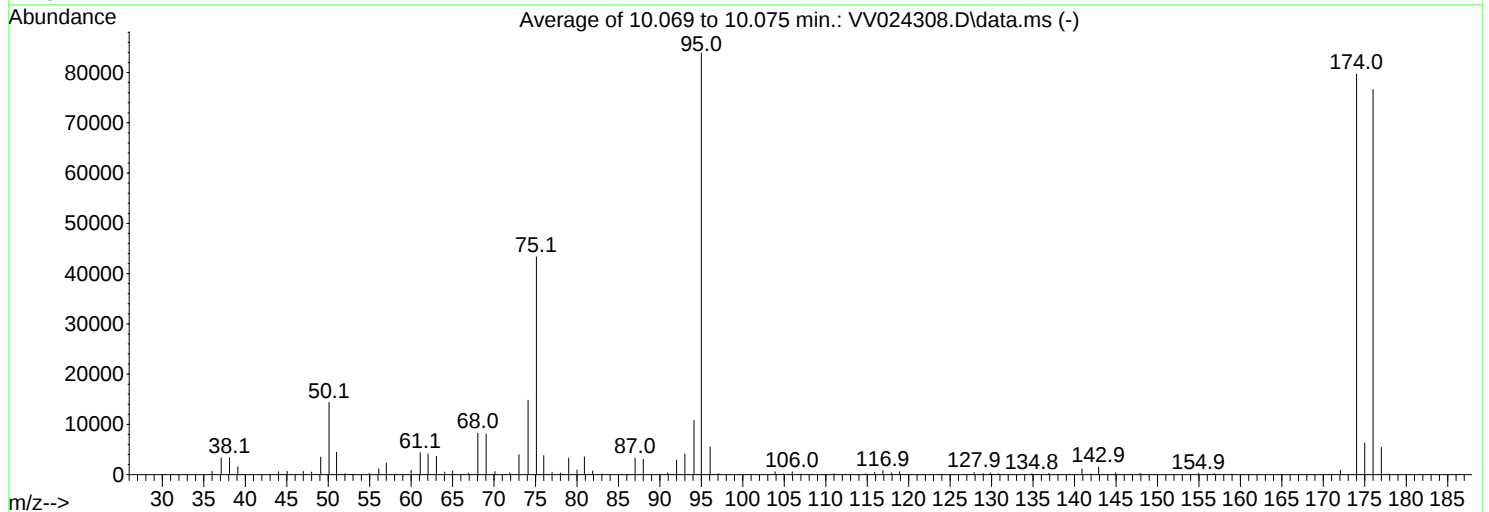


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV010822\
 Data File : VV024308.D
 Acq On : 08 Jan 2022 10:22
 Operator : SY/MD
 Sample : BFB261
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB261

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Jan 11 01:51:56 2022

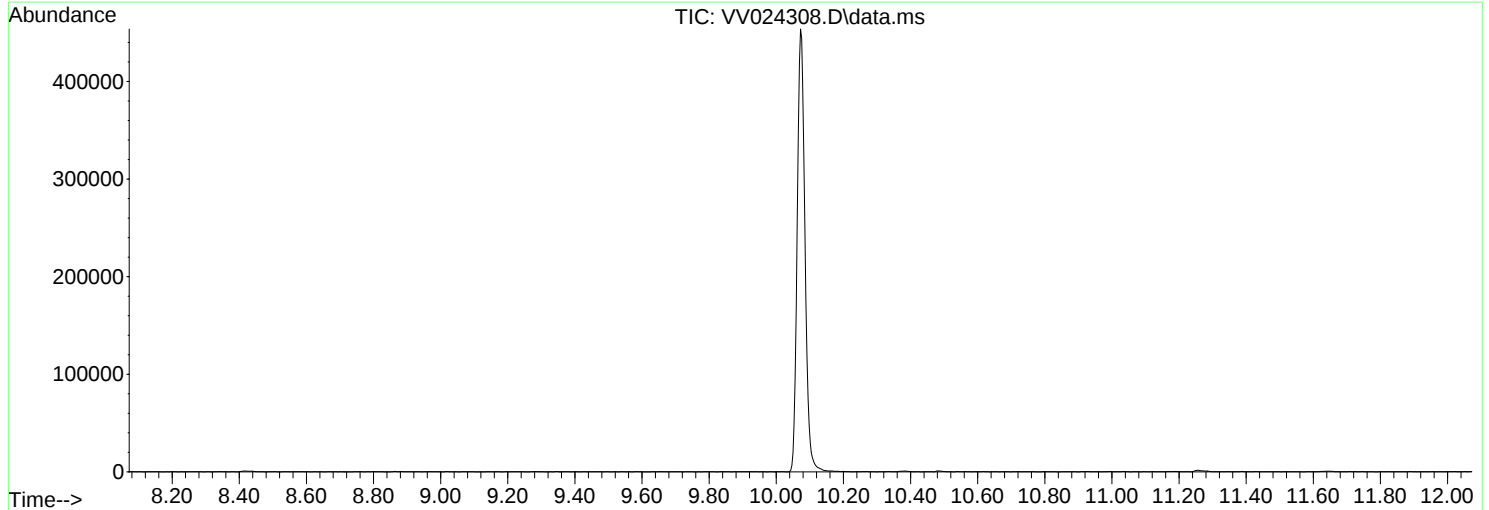

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	14378	PASS
75	95	30	80	51.6	43328	PASS
95	95	100	100	100.0	83931	PASS
96	95	5	9	6.5	5484	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.9	79680	PASS
175	174	5	9	7.9	6308	PASS
176	174	95	105	96.2	76637	PASS
177	176	5	10	7.1	5415	PASS

m/z	Abundance
36.00	643.0
37.10	3267.0
38.10	3423.0
39.10	1535.0
39.90	133.0
44.00	528.0
45.00	691.0
46.10	137.0
47.00	655.0
48.00	510.0
49.10	3265.0
50.10	13746.0
51.00	4281.0
52.00	212.0
54.90	263.0
56.10	1069.0
57.00	2333.0
60.00	953.0
61.10	4208.0
62.00	3941.0
63.00	3548.0
64.10	523.0
65.00	733.0
66.90	268.0
68.10	7980.0
69.00	7845.0
70.10	684.0
71.90	402.0
73.00	3870.0
74.10	14226.0
75.10	41624.0
76.00	3611.0
77.00	449.0
78.00	279.0
79.00	3214.0
80.00	950.0
80.90	3318.0
81.90	759.0
83.10	102.0
86.00	108.0
87.00	3319.0
88.00	3180.0
90.90	308.0
92.00	2783.0
93.00	3893.0
94.10	10393.0
95.00	81288.0
96.00	5450.0
97.10	177.0
103.90	477.0
104.90	154.0
106.00	531.0
107.00	109.0
111.00	192.0
114.80	136.0
115.90	397.0
116.90	768.0
117.90	327.0
118.90	544.0
123.70	104.0
127.90	395.0
129.00	222.0
129.90	295.0
130.80	169.0
135.00	219.0
136.90	208.0
140.90	1093.0
142.00	119.0
142.90	1270.0
145.00	416.0
145.80	113.0
146.80	132.0
148.00	243.0
149.90	110.0
154.90	229.0
156.80	201.0
159.00	135.0
171.00	171.0
172.10	809.0
174.00	74280.0
175.00	6133.0
176.00	71632.0
177.00	5186.0
177.90	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

m/z	Abundance
36.00	693.0
37.10	3499.0
38.10	3546.0
39.10	1652.0
39.90	112.0
44.00	585.0
45.10	720.0
46.10	118.0
47.00	634.0
48.00	513.0
49.10	3617.0
50.10	14848.0
51.00	4566.0
52.00	238.0
55.00	284.0
56.10	1197.0
57.00	2382.0
58.00	103.0
60.00	937.0
61.10	4610.0
62.10	4249.0
63.10	3726.0
64.10	543.0
65.00	778.0
66.90	338.0
68.10	8510.0
69.10	8278.0
70.10	632.0
71.90	403.0
73.00	4094.0
74.10	15290.0
75.10	44888.0
76.00	3917.0
77.00	461.0
78.00	329.0
79.00	3458.0
80.00	1005.0
80.90	3644.0
81.90	750.0
83.00	128.0
86.10	103.0
87.00	3408.0
88.00	3143.0
91.00	346.0
92.00	3042.0
93.00	4241.0
94.10	11161.0
95.00	87016.0
96.00	5642.0
97.10	220.0
103.90	577.0
104.90	202.0
105.90	597.0
107.00	144.0
111.00	186.0
114.80	164.0
115.90	492.0
116.90	839.0
117.90	366.0
118.90	580.0
127.90	475.0
129.00	252.0
129.80	356.0
130.80	187.0
134.80	193.0
136.90	247.0
139.90	110.0
140.90	1180.0
142.00	128.0
142.90	1541.0
144.90	400.0
145.80	120.0
146.80	132.0
147.90	231.0
155.00	244.0
156.90	203.0
158.90	151.0
171.20	196.0
172.10	889.0
174.00	82392.0
175.00	6460.0
176.00	79184.0
177.00	5583.0
177.90	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

m/z	Abundance
36.00	702.0
37.10	3325.0
38.10	3176.0
39.10	1551.0
44.00	639.0
45.00	628.0
47.00	611.0
48.00	471.0
49.10	3561.0
50.10	14540.0
51.00	4396.0
52.10	232.0
52.90	112.0
55.00	280.0
56.10	1296.0
57.00	2172.0
58.10	126.0
60.00	802.0
61.10	4324.0
62.00	4168.0
63.10	3650.0
64.00	513.0
65.00	716.0
67.00	384.0
68.00	8278.0
69.10	8150.0
70.10	551.0
71.90	345.0
73.00	3991.0
74.10	14924.0
75.10	43472.0
76.00	3814.0
77.00	446.0
78.00	342.0
79.00	3322.0
80.00	938.0
80.90	3612.0
81.90	709.0
83.00	128.0
87.00	3244.0
88.00	2875.0
91.00	368.0
92.00	2829.0
93.00	4192.0
94.10	10792.0
95.00	83488.0
96.10	5360.0
97.10	254.0
103.90	628.0
104.90	224.0
105.90	579.0
107.10	160.0
109.80	110.0
111.00	164.0
112.80	121.0
114.80	166.0
115.90	517.0
116.90	831.0
117.90	389.0
118.90	559.0
127.90	508.0
129.00	241.0
129.90	355.0
130.80	183.0
134.80	196.0
136.90	281.0
139.90	115.0
140.90	1136.0
142.00	128.0
142.90	1689.0
144.90	359.0
146.00	110.0
147.80	255.0
155.00	276.0
156.90	222.0
158.90	155.0
160.90	102.0
170.70	138.0
172.00	895.0
174.00	82368.0
175.00	6331.0
176.00	79096.0
177.00	5475.0
177.90	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261