

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033561.D
 Acq On : 10 Jan 2024 15:29
 Operator : SY/MD
 Sample : VV0110WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M

Title : VOC Analysis

Signal : TIC: VV033561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	191281	210440	15.63%	1.989%
2	2.053	306	315	328	rBV	300493	433268	32.17%	4.096%
3	2.767	535	537	541	rBV3	553	330	0.02%	0.003%
4	2.937	588	590	594	rBV3	771	466	0.03%	0.004%
5	3.285	697	698	703	rVB4	660	487	0.04%	0.005%
6	3.310	703	706	709	rBV4	603	504	0.04%	0.005%
7	3.436	743	745	747	rBV2	612	376	0.03%	0.004%
8	3.458	750	752	754	rBV3	468	225	0.02%	0.002%
9	3.613	797	800	801	rBV3	513	218	0.02%	0.002%
10	3.622	801	803	806	rVV	530	390	0.03%	0.004%
11	3.638	806	808	814	rVB5	669	565	0.04%	0.005%
12	3.667	815	817	820	rBV4	238	155	0.01%	0.001%
13	3.786	846	854	901	rBV	87730	265792	19.74%	2.513%
14	4.246	983	997	1026	rBV	198115	503643	37.40%	4.761%
15	4.564	1094	1096	1097	rBV2	643	308	0.02%	0.003%
16	4.693	1134	1136	1138	rBV2	377	183	0.01%	0.002%
17	4.738	1147	1150	1151	rBV2	348	227	0.02%	0.002%
18	4.828	1174	1178	1179	rBV2	538	414	0.03%	0.004%
19	4.883	1192	1195	1196	rBV	308	137	0.01%	0.001%
20	4.953	1200	1217	1252	rBV2	508874	1346759	100.00%	12.731%
21	5.487	1380	1383	1385	rBV4	527	257	0.02%	0.002%
22	5.532	1385	1397	1432	rBV	408736	850267	63.13%	8.038%
23	5.831	1480	1490	1502	rBV8	6988	16469	1.22%	0.156%
24	5.986	1526	1538	1576	rVB	293573	605728	44.98%	5.726%
25	6.301	1633	1636	1640	rBV4	557	492	0.04%	0.005%
26	6.381	1658	1661	1664	rBV3	327	189	0.01%	0.002%
27	6.494	1695	1696	1698	rBV2	425	174	0.01%	0.002%
28	6.561	1714	1717	1718	rBV2	513	247	0.02%	0.002%
29	6.574	1718	1721	1723	rVV3	651	401	0.03%	0.004%
30	6.744	1770	1774	1775	rBV2	320	231	0.02%	0.002%
31	6.754	1775	1777	1780	rVV3	339	216	0.02%	0.002%
32	6.777	1783	1784	1788	rBV2	514	265	0.02%	0.003%
33	6.860	1807	1810	1814	rVB3	388	257	0.02%	0.002%
34	6.912	1814	1826	1857	rBV	182890	342688	25.45%	3.240%
35	7.243	1918	1929	1956	rBV	611072	1080223	80.21%	10.212%
36	7.551	2016	2025	2053	rBV	126154	227367	16.88%	2.149%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033561.D
 Acq On : 10 Jan 2024 15:29
 Operator : SY/MD
 Sample : VV0110WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	7.850	2114	2118	2122	rVB5	466	367	0.03%	0.003%
38	7.876	2122	2126	2129	rBV5	452	461	0.03%	0.004%
39	7.915	2134	2138	2142	rVB3	1215	982	0.07%	0.009%
40	7.957	2146	2151	2154	rBV2	500	408	0.03%	0.004%
41	8.027	2163	2173	2217	rBV	350182	707103	52.50%	6.685%
42	8.657	2366	2369	2372	rBV4	340	147	0.01%	0.001%
43	8.674	2372	2374	2377	rVB3	436	244	0.02%	0.002%
44	8.690	2377	2379	2380	rBV3	473	247	0.02%	0.002%
45	8.744	2392	2396	2397	rBV4	690	486	0.04%	0.005%
46	8.783	2397	2408	2433	rVV	634164	1035319	76.87%	9.787%
47	9.072	2495	2498	2500	rBV4	954	693	0.05%	0.007%
48	9.188	2530	2534	2536	rVB4	567	429	0.03%	0.004%
49	9.204	2536	2539	2542	rBV4	656	502	0.04%	0.005%
50	9.288	2563	2565	2569	rBV3	484	390	0.03%	0.004%
51	9.320	2573	2575	2578	rVV	829	343	0.03%	0.003%
52	9.346	2578	2583	2586	rVB2	684	392	0.03%	0.004%
53	9.362	2586	2588	2591	rBV2	465	236	0.02%	0.002%
54	9.426	2605	2608	2610	rBV4	440	251	0.02%	0.002%
55	9.593	2657	2660	2661	rBV2	642	221	0.02%	0.002%
56	9.680	2684	2687	2689	rBV3	570	336	0.02%	0.003%
57	9.712	2695	2697	2699	rBV3	457	251	0.02%	0.002%
58	9.738	2702	2705	2708	rVB4	392	238	0.02%	0.002%
59	9.754	2708	2710	2713	rBV	317	149	0.01%	0.001%
60	9.873	2737	2747	2756	rBV5	2741	4495	0.33%	0.042%
61	9.947	2767	2770	2772	rBV3	431	289	0.02%	0.003%
62	9.979	2776	2780	2781	rBV4	360	274	0.02%	0.003%
63	10.001	2786	2787	2791	rVB2	533	327	0.02%	0.003%
64	10.024	2791	2794	2795	rBV3	243	146	0.01%	0.001%
65	10.034	2795	2797	2800	rBV3	267	160	0.01%	0.002%
66	10.053	2800	2803	2807	rBV4	543	311	0.02%	0.003%
67	10.079	2809	2811	2814	rVB2	534	324	0.02%	0.003%
68	10.098	2814	2817	2818	rBV2	455	265	0.02%	0.003%
69	10.156	2819	2835	2854	rBV	380921	624045	46.34%	5.899%
70	10.413	2912	2915	2916	rBV2	294	133	0.01%	0.001%
71	10.484	2928	2937	2948	rVV3	2826	4667	0.35%	0.044%
72	10.645	2984	2987	2988	rBV2	479	238	0.02%	0.002%
73	10.960	3082	3085	3087	rBV2	307	234	0.02%	0.002%
74	10.973	3087	3089	3093	rVB3	409	245	0.02%	0.002%
75	11.014	3099	3102	3103	rBV4	399	259	0.02%	0.002%
76	11.085	3123	3124	3128	rBV2	356	227	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033561.D
 Acq On : 10 Jan 2024 15:29
 Operator : SY/MD
 Sample : VV0110WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.130	3128	3138	3144	rBV4	4920	7615	0.57%	0.072%
78	11.185	3145	3155	3178	rVV	692134	1095201	81.32%	10.353%
79	11.378	3212	3215	3219	rBV5	561	449	0.03%	0.004%
80	11.471	3241	3244	3245	rBV3	354	174	0.01%	0.002%
81	11.513	3255	3257	3261	rBV	370	247	0.02%	0.002%
82	11.561	3261	3272	3296	rBV	637087	1023676	76.01%	9.677%
83	11.837	3354	3358	3360	rBV3	1013	582	0.04%	0.006%
84	11.972	3398	3400	3403	rBV2	318	195	0.01%	0.002%
85	12.014	3411	3413	3414	rBV2	378	155	0.01%	0.001%
86	12.111	3441	3443	3445	rBV2	397	165	0.01%	0.002%
87	12.554	3578	3581	3583	rVB3	356	198	0.01%	0.002%
88	12.590	3583	3592	3603	rBV4	8457	13218	0.98%	0.125%
89	12.670	3614	3617	3620	rBV3	284	255	0.02%	0.002%
90	12.718	3629	3632	3633	rBV3	508	278	0.02%	0.003%
91	12.873	3676	3680	3681	rBV2	345	229	0.02%	0.002%
92	12.956	3702	3706	3709	rVB6	558	426	0.03%	0.004%
93	12.979	3709	3713	3714	rBV2	545	393	0.03%	0.004%
94	13.053	3732	3736	3738	rBV3	788	645	0.05%	0.006%
95	13.130	3756	3760	3764	rBV5	443	423	0.03%	0.004%
96	13.204	3775	3783	3795	rBV2	16069	26175	1.94%	0.247%
97	13.288	3805	3809	3813	rBV4	937	774	0.06%	0.007%
98	13.445	3848	3858	3877	rBV	55069	96642	7.18%	0.914%
99	13.686	3924	3933	3943	rBV2	20792	32285	2.40%	0.305%
100	13.857	3982	3986	3990	rVB4	708	634	0.05%	0.006%




Sum of corrected areas: 10578226

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033561.D
Acq On : 10 Jan 2024 15:29
Operator : SY/MD
Sample : VV0110WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

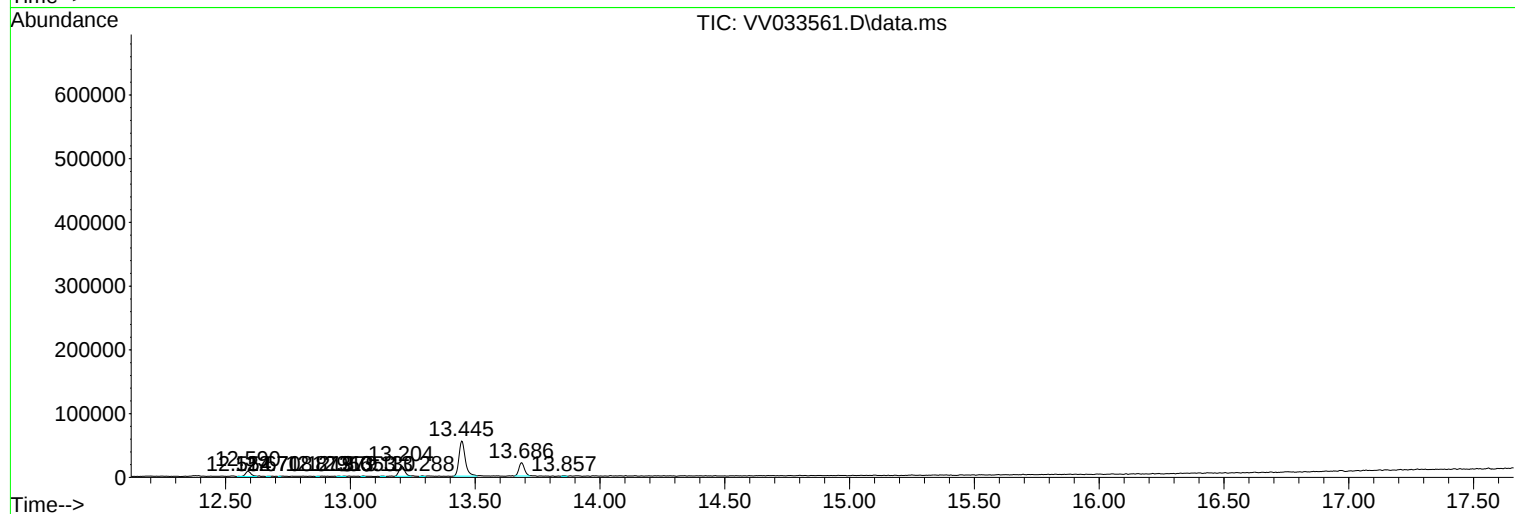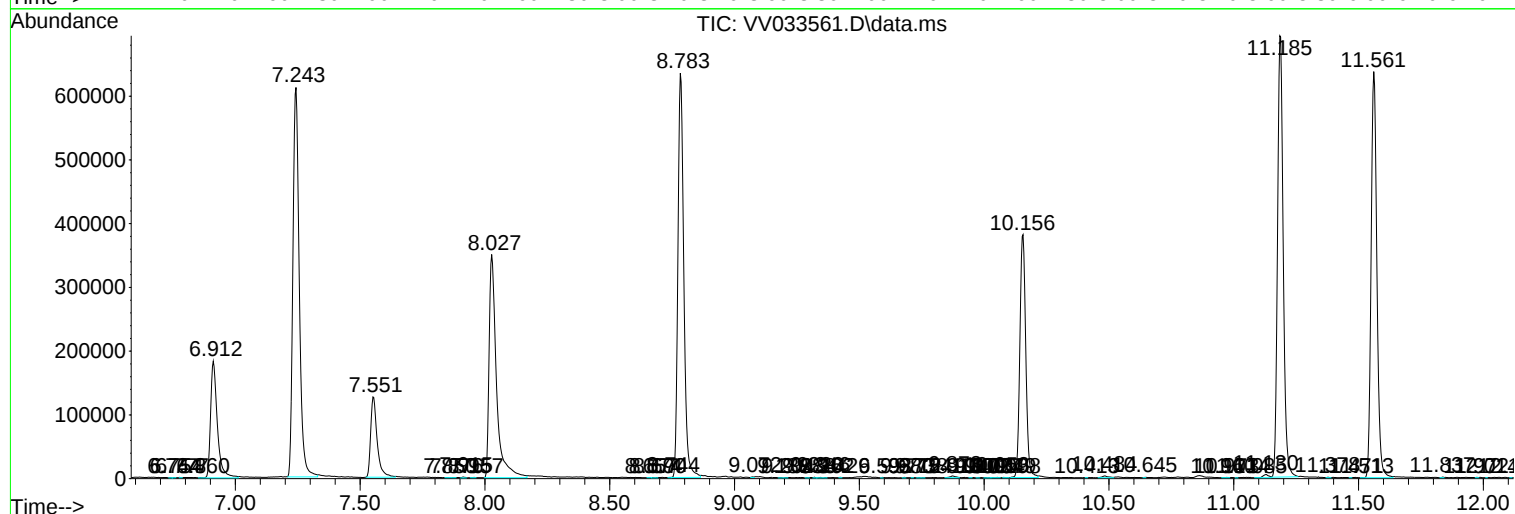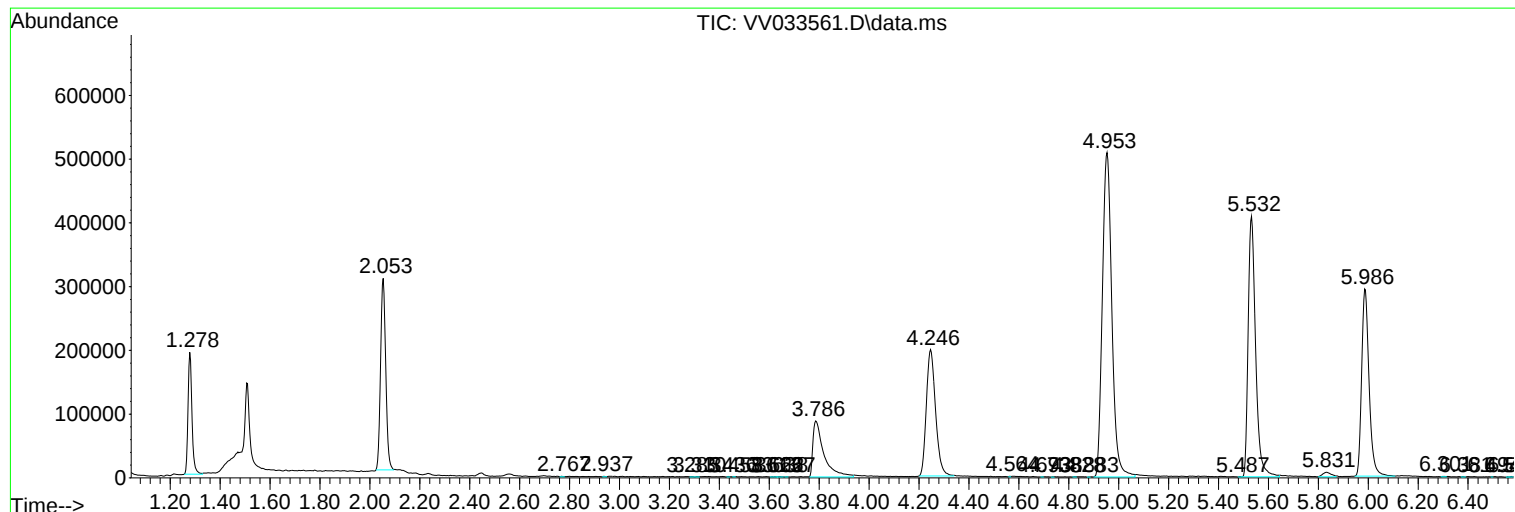

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033561.D
Acq On : 10 Jan 2024 15:29
Operator : SY/MD
Sample : VV0110WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033561.D
Acq On : 10 Jan 2024 15:29
Operator : SY/MD
Sample : VV0110WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------