

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033567.D
 Acq On : 10 Jan 2024 17:54
 Operator : SY/MD
 Sample : P1061-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	33	39	44	rBV	1906	2274	0.17%	0.023%
2	1.278	67	74	88	rBV	189162	199269	15.33%	2.009%
3	1.529	145	152	168	rVB	144150	173772	13.37%	1.752%
4	2.060	307	317	332	rBV	289993	422561	32.50%	4.261%
5	2.445	433	437	438	rBV4	1140	700	0.05%	0.007%
6	2.622	489	492	494	rBV3	497	372	0.03%	0.004%
7	3.278	691	696	698	rBV4	432	385	0.03%	0.004%
8	3.654	808	813	815	rVB4	439	369	0.03%	0.004%
9	3.703	821	828	830	rBV6	449	397	0.03%	0.004%
10	3.716	830	832	836	rVB3	489	379	0.03%	0.004%
11	3.748	836	842	844	rBV3	522	460	0.04%	0.005%
12	3.783	844	853	893	rBV	95209	259785	19.98%	2.620%
13	4.124	957	959	962	rBV2	570	366	0.03%	0.004%
14	4.249	980	998	1030	rBV	191182	497065	38.24%	5.012%
15	4.394	1040	1043	1044	rBV	673	431	0.03%	0.004%
16	4.751	1151	1154	1156	rBV3	649	415	0.03%	0.004%
17	4.815	1170	1174	1177	rBV4	501	332	0.03%	0.003%
18	4.957	1199	1218	1255	rBV2	489213	1300002	100.00%	13.109%
19	5.256	1309	1311	1313	rBV3	687	375	0.03%	0.004%
20	5.535	1386	1398	1427	rBV	387522	803865	61.84%	8.106%
21	5.831	1480	1490	1510	rVB4	7872	18117	1.39%	0.183%
22	5.989	1525	1539	1567	rBV	285316	594948	45.77%	5.999%
23	6.313	1638	1640	1646	rBV6	502	523	0.04%	0.005%
24	6.439	1676	1679	1681	rVV3	576	329	0.03%	0.003%
25	6.465	1685	1687	1693	rVB4	588	423	0.03%	0.004%
26	6.593	1724	1727	1730	rBV4	494	426	0.03%	0.004%
27	6.757	1773	1778	1779	rBV3	366	339	0.03%	0.003%
28	6.915	1812	1827	1856	rBV	168920	320792	24.68%	3.235%
29	7.140	1895	1897	1900	rBV3	565	344	0.03%	0.003%
30	7.243	1918	1929	1962	rBV	586431	1034785	79.60%	10.434%
31	7.555	2016	2026	2056	rBV	115822	211439	16.26%	2.132%
32	7.715	2074	2076	2079	rVB3	714	313	0.02%	0.003%
33	7.805	2101	2104	2111	rVB5	550	651	0.05%	0.007%
34	7.873	2121	2125	2140	rVB3	2545	4367	0.34%	0.044%
35	8.024	2162	2172	2217	rBV	336890	654953	50.38%	6.604%
36	8.439	2297	2301	2305	rBV4	563	572	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033567.D
 Acq On : 10 Jan 2024 17:54
 Operator : SY/MD
 Sample : P1061-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	8.503	2318	2321	2323	rBV4	700	410	0.03%	0.004%
38	8.564	2337	2340	2344	rBV3	731	682	0.05%	0.007%
39	8.722	2387	2389	2398	rVB6	759	726	0.06%	0.007%
40	8.786	2398	2409	2438	rBV	581640	975871	75.07%	9.840%
41	9.284	2559	2564	2566	rBV3	455	421	0.03%	0.004%
42	9.378	2590	2593	2597	rVB3	479	389	0.03%	0.004%
43	9.452	2612	2616	2618	rBV3	513	347	0.03%	0.003%
44	9.490	2624	2628	2632	rVB3	494	378	0.03%	0.004%
45	9.519	2632	2637	2640	rBV3	810	587	0.05%	0.006%
46	9.667	2678	2683	2686	rBV5	550	470	0.04%	0.005%
47	9.715	2691	2698	2700	rBV5	645	633	0.05%	0.006%
48	9.799	2720	2724	2729	rVB4	836	643	0.05%	0.006%
49	9.924	2757	2763	2766	rBV4	525	496	0.04%	0.005%
50	10.001	2782	2787	2793	rVB7	521	621	0.05%	0.006%
51	10.040	2796	2799	2804	rVB3	425	320	0.02%	0.003%
52	10.088	2811	2814	2819	rVB4	463	357	0.03%	0.004%
53	10.153	2819	2834	2859	rBV	357434	565065	43.47%	5.698%
54	10.259	2863	2867	2870	rBV3	673	561	0.04%	0.006%
55	10.329	2880	2889	2894	rVB3	2350	3197	0.25%	0.032%
56	10.474	2932	2934	2938	rBV4	377	311	0.02%	0.003%
57	10.532	2947	2952	2953	rBV3	835	493	0.04%	0.005%
58	10.616	2975	2978	2983	rVB4	460	421	0.03%	0.004%
59	10.680	2995	2998	3001	rBV2	503	412	0.03%	0.004%
60	10.786	3027	3031	3034	rVB4	526	402	0.03%	0.004%
61	10.808	3035	3038	3044	rVB4	707	599	0.05%	0.006%
62	10.921	3067	3073	3074	rBV2	629	536	0.04%	0.005%
63	11.011	3095	3101	3103	rVB3	469	425	0.03%	0.004%
64	11.059	3114	3116	3118	rBV3	586	332	0.03%	0.003%
65	11.127	3131	3137	3138	rBV4	680	490	0.04%	0.005%
66	11.185	3144	3155	3182	rBV	594828	929923	71.53%	9.377%
67	11.300	3190	3191	3196	rVB4	568	387	0.03%	0.004%
68	11.423	3226	3229	3233	rBB3	519	352	0.03%	0.004%
69	11.561	3258	3272	3300	rVV	573988	902099	69.39%	9.096%
70	11.731	3322	3325	3330	rVB4	586	490	0.04%	0.005%
71	11.757	3331	3333	3338	rVB6	642	478	0.04%	0.005%
72	11.780	3338	3340	3343	rBV3	582	323	0.02%	0.003%
73	11.828	3353	3355	3359	rVB4	476	350	0.03%	0.004%
74	11.886	3368	3373	3375	rBV3	680	471	0.04%	0.005%
75	12.066	3426	3429	3433	rBV5	429	405	0.03%	0.004%
76	12.124	3444	3447	3450	rBV2	370	324	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033567.D
 Acq On : 10 Jan 2024 17:54
 Operator : SY/MD
 Sample : P1061-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.172	3459	3462	3465	rBV2	503	350	0.03%	0.004%
78	12.310	3501	3505	3509	rBV4	379	380	0.03%	0.004%
79	12.516	3565	3569	3571	rBV4	479	353	0.03%	0.004%
80	12.564	3579	3584	3585	rBV2	401	321	0.02%	0.003%
81	12.779	3646	3651	3657	rBV6	480	595	0.05%	0.006%
82	12.808	3657	3660	3664	rVV4	469	407	0.03%	0.004%
83	12.905	3687	3690	3694	rBV4	628	399	0.03%	0.004%
84	12.943	3697	3702	3705	rBV5	528	450	0.03%	0.005%
85	13.037	3727	3731	3736	rBV3	770	712	0.05%	0.007%
86	13.104	3748	3752	3755	rBV4	518	520	0.04%	0.005%
87	13.162	3767	3770	3775	rVB3	515	352	0.03%	0.004%
88	13.210	3778	3785	3793	rBV7	2068	3089	0.24%	0.031%
89	13.265	3798	3802	3806	rVB3	495	506	0.04%	0.005%
90	13.291	3806	3810	3812	rBV4	535	382	0.03%	0.004%
91	13.355	3826	3830	3833	rBV4	616	503	0.04%	0.005%
92	13.410	3844	3847	3851	rBV4	691	709	0.05%	0.007%
93	13.451	3851	3860	3861	rBV6	3263	3014	0.23%	0.030%
94	13.548	3887	3890	3892	rBV3	640	388	0.03%	0.004%
95	13.664	3921	3926	3929	rBV4	729	706	0.05%	0.007%
96	13.686	3929	3933	3938	rBV5	1152	1198	0.09%	0.012%
97	14.027	4035	4039	4044	rBV5	825	847	0.07%	0.009%
98	14.133	4068	4072	4076	rBV3	550	530	0.04%	0.005%
99	14.159	4077	4080	4085	rBV4	437	468	0.04%	0.005%
100	15.168	4390	4394	4396	rBV2	880	745	0.06%	0.008%




Sum of corrected areas: 9917016

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033567.D
Acq On : 10 Jan 2024 17:54
Operator : SY/MD
Sample : P1061-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

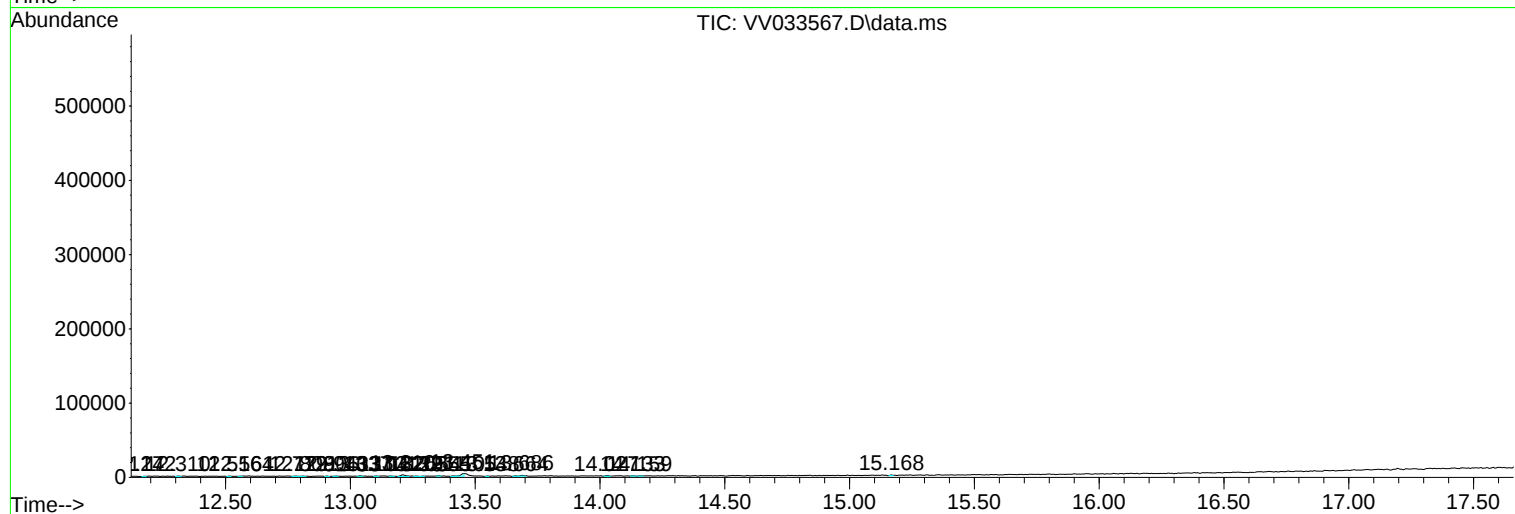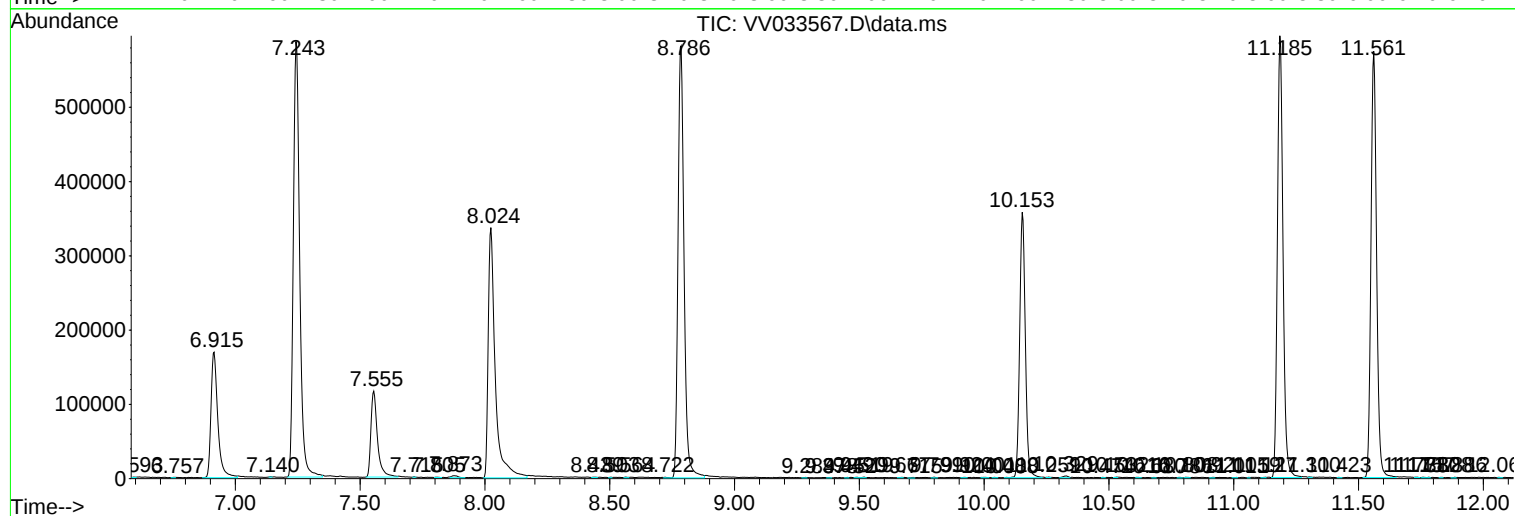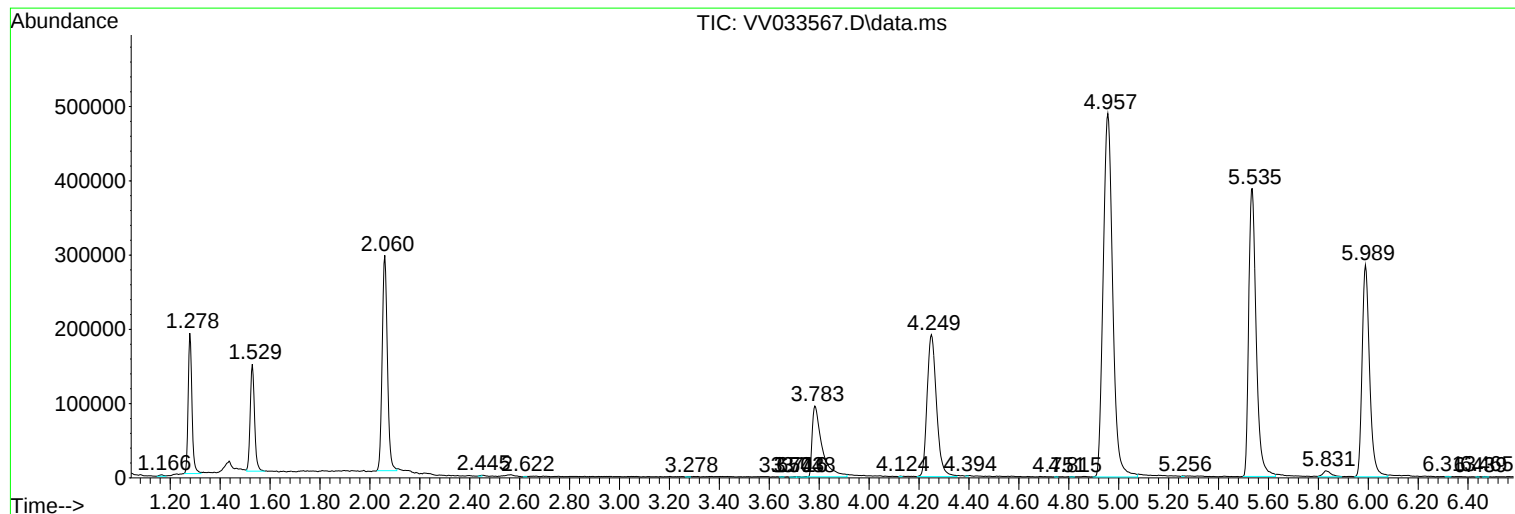

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033567.D
Acq On : 10 Jan 2024 17:54
Operator : SY/MD
Sample : P1061-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033567.D
Acq On : 10 Jan 2024 17:54
Operator : SY/MD
Sample : P1061-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc