

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033569.D
 Acq On : 10 Jan 2024 18:42
 Operator : SY/MD
 Sample : P1061-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033569.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	29	rVB2	23629	26739	2.01%	0.261%
2	1.278	67	74	88	rBV	203408	217018	16.29%	2.121%
3	1.529	146	152	166	rVB	143178	175537	13.17%	1.716%
4	2.060	308	317	331	rBV	294072	426324	32.00%	4.167%
5	2.700	506	516	521	rBV6	1134	2194	0.16%	0.021%
6	2.764	533	536	539	rBV3	596	427	0.03%	0.004%
7	2.796	543	546	548	rBV3	585	461	0.03%	0.005%
8	3.288	695	699	701	rBV3	338	270	0.02%	0.003%
9	3.365	720	723	725	rBV3	333	242	0.02%	0.002%
10	3.494	760	763	764	rBV3	383	193	0.01%	0.002%
11	3.539	771	777	779	rBV2	482	411	0.03%	0.004%
12	3.574	785	788	789	rBV3	309	181	0.01%	0.002%
13	3.622	800	803	807	rBV4	501	460	0.03%	0.004%
14	3.664	814	816	818	rBV2	278	188	0.01%	0.002%
15	3.732	833	837	840	rBV5	255	258	0.02%	0.003%
16	3.783	845	853	891	rBV	90029	248293	18.64%	2.427%
17	4.249	983	998	1027	rBV	197640	505436	37.93%	4.941%
18	4.722	1141	1145	1146	rBV3	307	232	0.02%	0.002%
19	4.809	1169	1172	1174	rBV2	788	556	0.04%	0.005%
20	4.902	1195	1201	1202	rBV4	295	288	0.02%	0.003%
21	4.957	1202	1218	1250	rBV2	501527	1332386	100.00%	13.024%
22	5.400	1354	1356	1358	rBV3	634	254	0.02%	0.002%
23	5.532	1386	1397	1437	rBV	412699	855268	64.19%	8.360%
24	5.834	1482	1491	1504	rVB10	3662	8540	0.64%	0.083%
25	5.944	1522	1525	1526	rBV2	590	363	0.03%	0.004%
26	5.989	1526	1539	1567	rVV	297390	610115	45.79%	5.964%
27	6.490	1690	1695	1697	rBV4	342	312	0.02%	0.003%
28	6.661	1746	1748	1750	rBV2	294	156	0.01%	0.002%
29	6.802	1787	1792	1795	rBV6	386	323	0.02%	0.003%
30	6.818	1795	1797	1800	rBV	398	232	0.02%	0.002%
31	6.867	1806	1812	1813	rBV4	404	366	0.03%	0.004%
32	6.912	1816	1826	1854	rBV	172308	324940	24.39%	3.176%
33	7.243	1918	1929	1954	rBV	596407	1060594	79.60%	10.367%
34	7.555	2016	2026	2055	rBV	115111	214172	16.07%	2.093%
35	7.854	2117	2119	2120	rBV	467	215	0.02%	0.002%
36	7.969	2152	2155	2160	rBV3	399	299	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033569.D
 Acq On : 10 Jan 2024 18:42
 Operator : SY/MD
 Sample : P1061-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	8.024	2162	2172	2211	rBV	333724	638990	47.96%	6.246%
38	8.477	2310	2313	2315	rBV3	425	256	0.02%	0.003%
39	8.632	2359	2361	2366	rVB4	530	325	0.02%	0.003%
40	8.658	2366	2369	2371	rBV2	475	339	0.03%	0.003%
41	8.719	2384	2388	2391	rBV4	642	518	0.04%	0.005%
42	8.783	2397	2408	2434	rBV	627588	1027436	77.11%	10.043%
43	9.140	2517	2519	2521	rBV2	431	238	0.02%	0.002%
44	9.211	2538	2541	2544	rVB2	437	257	0.02%	0.003%
45	9.230	2544	2547	2550	rBV2	237	207	0.02%	0.002%
46	9.336	2575	2580	2581	rBV3	350	278	0.02%	0.003%
47	9.371	2588	2591	2594	rBV4	491	403	0.03%	0.004%
48	9.439	2609	2612	2614	rBV2	423	306	0.02%	0.003%
49	9.484	2623	2626	2627	rBV2	427	216	0.02%	0.002%
50	9.545	2642	2645	2649	rBV4	536	446	0.03%	0.004%
51	9.603	2660	2663	2665	rBV2	559	324	0.02%	0.003%
52	9.632	2669	2672	2674	rBV4	722	523	0.04%	0.005%
53	9.677	2683	2686	2689	rVB3	389	291	0.02%	0.003%
54	9.719	2695	2699	2701	rBV4	712	554	0.04%	0.005%
55	9.982	2778	2781	2783	rBV2	447	298	0.02%	0.003%
56	10.034	2792	2797	2800	rBV4	551	485	0.04%	0.005%
57	10.153	2819	2834	2860	rBV	365341	585562	43.95%	5.724%
58	10.329	2884	2889	2895	rVB5	1258	1530	0.11%	0.015%
59	10.362	2897	2899	2903	rBV4	423	255	0.02%	0.002%
60	10.391	2906	2908	2911	rVB3	482	194	0.01%	0.002%
61	10.442	2920	2924	2927	rBV3	486	446	0.03%	0.004%
62	10.596	2966	2972	2977	rBV5	442	520	0.04%	0.005%
63	10.674	2987	2996	3002	rVB7	1053	1922	0.14%	0.019%
64	10.802	3033	3036	3037	rBV2	531	219	0.02%	0.002%
65	10.863	3049	3055	3057	rBV5	798	890	0.07%	0.009%
66	10.911	3065	3070	3071	rBV4	519	482	0.04%	0.005%
67	11.005	3097	3099	3101	rBV	317	176	0.01%	0.002%
68	11.050	3111	3113	3115	rBV	451	306	0.02%	0.003%
69	11.098	3123	3128	3130	rBV5	875	842	0.06%	0.008%
70	11.140	3139	3141	3142	rBV2	485	214	0.02%	0.002%
71	11.185	3144	3155	3183	rVV	634830	1000488	75.09%	9.780%
72	11.464	3240	3242	3244	rBV3	353	172	0.01%	0.002%
73	11.561	3260	3272	3291	rBV	599309	940277	70.57%	9.191%
74	11.773	3334	3338	3341	rBV3	363	342	0.03%	0.003%
75	11.937	3386	3389	3392	rVB4	351	170	0.01%	0.002%
76	11.966	3396	3398	3402	rBV2	346	221	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033569.D
 Acq On : 10 Jan 2024 18:42
 Operator : SY/MD
 Sample : P1061-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCMJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.030	3416	3418	3420	rBV	306	166	0.01%	0.002%
78	12.085	3431	3435	3437	rBV4	615	539	0.04%	0.005%
79	12.114	3440	3444	3448	rVB5	645	448	0.03%	0.004%
80	12.175	3457	3463	3466	rBV6	679	660	0.05%	0.006%
81	12.641	3607	3608	3611	rVB3	310	167	0.01%	0.002%
82	12.712	3628	3630	3633	rVB3	391	232	0.02%	0.002%
83	12.728	3633	3635	3637	rBV2	343	204	0.02%	0.002%
84	12.770	3646	3648	3654	rVB2	581	406	0.03%	0.004%
85	12.799	3654	3657	3658	rBV2	420	265	0.02%	0.003%
86	12.866	3675	3678	3679	rBV2	472	255	0.02%	0.002%
87	12.902	3687	3689	3692	rBV3	437	269	0.02%	0.003%
88	12.995	3715	3718	3719	rBV3	636	340	0.03%	0.003%
89	13.059	3735	3738	3742	rBV2	310	300	0.02%	0.003%
90	13.140	3760	3763	3766	rBV3	467	355	0.03%	0.003%
91	13.300	3810	3813	3816	rBV2	578	338	0.03%	0.003%
92	13.313	3816	3817	3821	rBV3	277	197	0.01%	0.002%
93	13.381	3834	3838	3839	rBV3	428	264	0.02%	0.003%
94	13.609	3907	3909	3910	rBV2	599	291	0.02%	0.003%
95	13.715	3940	3942	3945	rBV3	417	352	0.03%	0.003%
96	13.892	3995	3997	3999	rBV2	451	292	0.02%	0.003%
97	13.937	4009	4011	4012	rBV	495	219	0.02%	0.002%
98	13.995	4027	4029	4031	rBV2	595	403	0.03%	0.004%
99	14.050	4044	4046	4050	rBV3	791	524	0.04%	0.005%
100	14.088	4055	4058	4062	rBV3	983	752	0.06%	0.007%




Sum of corrected areas: 10230399

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033569.D
Acq On : 10 Jan 2024 18:42
Operator : SY/MD
Sample : P1061-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

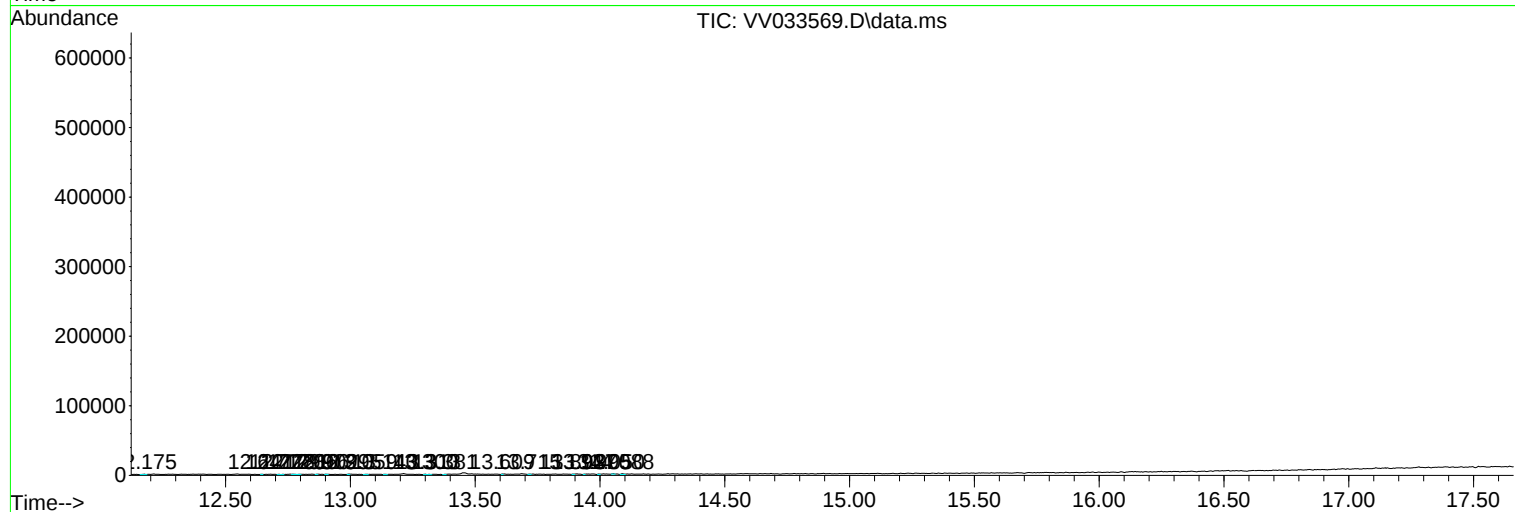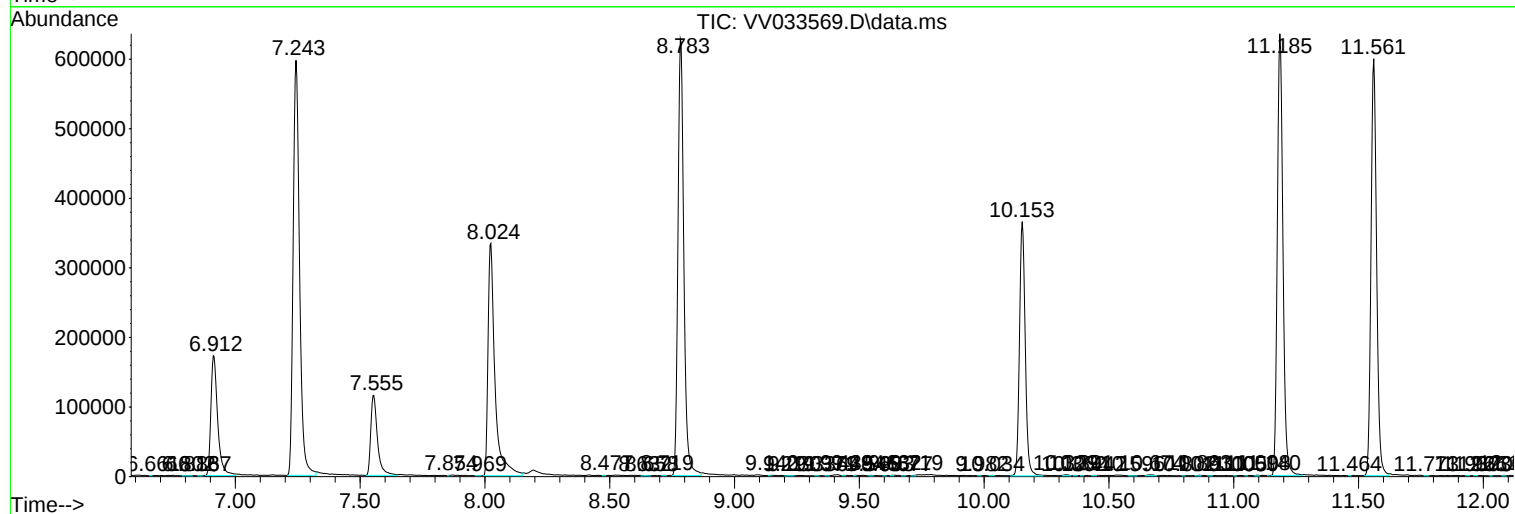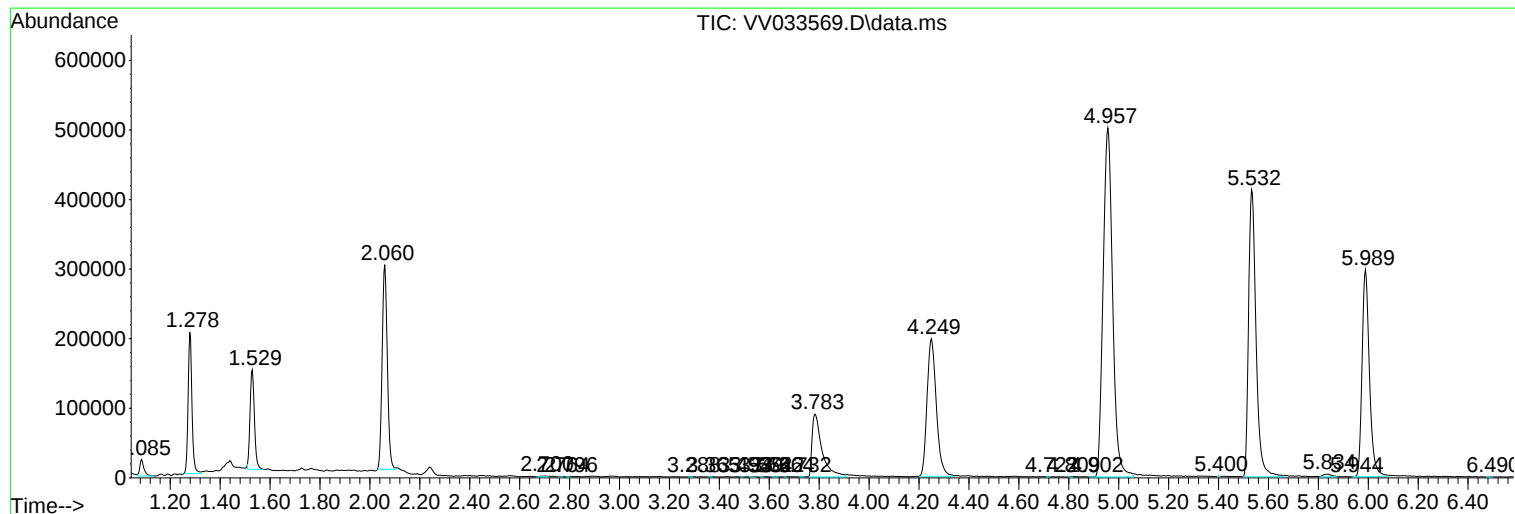

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033569.D
Acq On : 10 Jan 2024 18:42
Operator : SY/MD
Sample : P1061-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033569.D
Acq On : 10 Jan 2024 18:42
Operator : SY/MD
Sample : P1061-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCMJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------