

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033570.D
 Acq On : 10 Jan 2024 19:06
 Operator : SY/MD
 Sample : P1061-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	34	39	45	rBV	6657	6758	0.53%	0.069%
2	1.278	67	74	89	rBV	180063	191949	15.15%	1.971%
3	1.529	145	152	173	rVB	142676	177042	13.98%	1.818%
4	2.060	307	317	351	rVB	288648	446464	35.24%	4.584%
5	2.606	484	487	490	rBV2	567	496	0.04%	0.005%
6	2.773	537	539	545	rVB4	627	636	0.05%	0.007%
7	3.207	669	674	677	rBV4	467	428	0.03%	0.004%
8	3.371	720	725	726	rBV2	520	346	0.03%	0.004%
9	3.471	752	756	758	rBV4	500	359	0.03%	0.004%
10	3.564	779	785	790	rVB5	696	800	0.06%	0.008%
11	3.619	800	802	806	rVB3	452	306	0.02%	0.003%
12	3.661	810	815	819	rVV4	551	464	0.04%	0.005%
13	3.748	837	842	844	rBV3	607	501	0.04%	0.005%
14	3.783	844	853	889	rBV	92408	249210	19.67%	2.559%
15	4.249	978	998	1026	rBV	188272	486532	38.40%	4.995%
16	4.683	1129	1133	1134	rBV3	491	347	0.03%	0.004%
17	4.693	1134	1136	1141	rVV2	513	307	0.02%	0.003%
18	4.754	1152	1155	1161	rVB3	630	606	0.05%	0.006%
19	4.802	1163	1170	1173	rVB4	542	635	0.05%	0.007%
20	4.957	1201	1218	1250	rBV2	477352	1266847	100.00%	13.007%
21	5.288	1318	1321	1323	rBV2	738	449	0.04%	0.005%
22	5.336	1333	1336	1339	rBV3	610	538	0.04%	0.006%
23	5.429	1362	1365	1371	rVB5	939	912	0.07%	0.009%
24	5.471	1376	1378	1384	rVB3	472	328	0.03%	0.003%
25	5.535	1386	1398	1437	rBV	385225	799360	63.10%	8.207%
26	5.764	1466	1469	1472	rBV4	657	539	0.04%	0.006%
27	5.834	1482	1491	1508	rBV3	5919	12174	0.96%	0.125%
28	5.989	1526	1539	1566	rBV	280566	584942	46.17%	6.006%
29	6.355	1650	1653	1659	rVB4	725	744	0.06%	0.008%
30	6.397	1659	1666	1669	rBV6	724	843	0.07%	0.009%
31	6.458	1682	1685	1688	rBV2	822	605	0.05%	0.006%
32	6.497	1695	1697	1702	rVB2	651	411	0.03%	0.004%
33	6.529	1703	1707	1712	rVB3	406	344	0.03%	0.004%
34	6.619	1732	1735	1741	rVB6	1096	1118	0.09%	0.011%
35	6.664	1745	1749	1751	rVB2	556	400	0.03%	0.004%
36	6.850	1803	1807	1810	rBV4	504	345	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033570.D
 Acq On : 10 Jan 2024 19:06
 Operator : SY/MD
 Sample : P1061-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	6.915	1813	1827	1853	rBV	164809	309259	24.41%	3.175%
38	7.243	1918	1929	1963	rBV	571912	1015105	80.13%	10.422%
39	7.555	2016	2026	2058	rBV	110144	200615	15.84%	2.060%
40	7.844	2112	2116	2118	rBV	564	393	0.03%	0.004%
41	7.918	2135	2139	2142	rBV3	478	476	0.04%	0.005%
42	7.950	2145	2149	2154	rVB5	555	647	0.05%	0.007%
43	7.979	2154	2158	2160	rBV2	592	361	0.03%	0.004%
44	8.024	2163	2172	2207	rBV	331495	630538	49.77%	6.474%
45	8.381	2278	2283	2289	rVB4	585	852	0.07%	0.009%
46	8.413	2289	2293	2298	rBV6	844	954	0.08%	0.010%
47	8.661	2366	2370	2376	rVB4	662	692	0.05%	0.007%
48	8.699	2376	2382	2386	rBV4	501	513	0.04%	0.005%
49	8.783	2398	2408	2442	rBV	573272	958405	75.65%	9.840%
50	9.066	2492	2496	2497	rBV3	599	400	0.03%	0.004%
51	9.133	2512	2517	2520	rBV3	482	428	0.03%	0.004%
52	9.265	2555	2558	2563	rVB6	514	411	0.03%	0.004%
53	9.297	2563	2568	2571	rBV4	583	548	0.04%	0.006%
54	9.416	2602	2605	2609	rVB4	462	342	0.03%	0.004%
55	9.551	2644	2647	2650	rVB3	730	453	0.04%	0.005%
56	9.574	2650	2654	2657	rBV4	593	502	0.04%	0.005%
57	9.960	2770	2774	2777	rBV4	382	333	0.03%	0.003%
58	10.066	2803	2807	2808	rBV2	385	314	0.02%	0.003%
59	10.104	2814	2819	2820	rBV3	396	304	0.02%	0.003%
60	10.153	2822	2834	2859	rVV	352881	553163	43.66%	5.679%
61	10.326	2884	2888	2889	rBV2	712	485	0.04%	0.005%
62	10.384	2904	2906	2914	rBV6	460	537	0.04%	0.006%
63	10.497	2939	2941	2944	rVB2	528	302	0.02%	0.003%
64	10.522	2944	2949	2952	rBV5	551	497	0.04%	0.005%
65	10.542	2953	2955	2962	rVB7	684	683	0.05%	0.007%
66	10.644	2982	2987	2989	rBV3	419	406	0.03%	0.004%
67	10.870	3051	3057	3059	rBV5	538	510	0.04%	0.005%
68	10.940	3075	3079	3083	rBV5	651	655	0.05%	0.007%
69	10.985	3087	3093	3095	rBV4	517	455	0.04%	0.005%
70	11.185	3144	3155	3178	rBV	597002	922589	72.83%	9.472%
71	11.561	3260	3272	3298	rVV	561783	886192	69.95%	9.098%
72	11.654	3298	3301	3306	rBV5	704	789	0.06%	0.008%
73	11.860	3360	3365	3368	rBV3	407	471	0.04%	0.005%
74	11.924	3379	3385	3388	rBV5	551	512	0.04%	0.005%
75	11.947	3388	3392	3395	rBV3	331	321	0.03%	0.003%
76	12.075	3428	3432	3434	rVB4	673	479	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033570.D
 Acq On : 10 Jan 2024 19:06
 Operator : SY/MD
 Sample : P1061-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	12.095	3434	3438	3440	rBV2	760	665	0.05%	0.007%
78	12.271	3488	3493	3497	rBV5	522	659	0.05%	0.007%
79	12.339	3512	3514	3520	rVB6	456	411	0.03%	0.004%
80	12.500	3562	3564	3570	rVB3	435	360	0.03%	0.004%
81	12.529	3570	3573	3576	rBV3	486	377	0.03%	0.004%
82	12.596	3588	3594	3596	rBV3	501	598	0.05%	0.006%
83	12.705	3624	3628	3630	rVB4	458	318	0.03%	0.003%
84	12.828	3661	3666	3667	rBV2	521	408	0.03%	0.004%
85	12.886	3681	3684	3688	rBV2	595	510	0.04%	0.005%
86	13.037	3725	3731	3734	rBV3	555	642	0.05%	0.007%
87	13.107	3750	3753	3755	rVB4	509	330	0.03%	0.003%
88	13.143	3757	3764	3769	rBV7	588	777	0.06%	0.008%
89	13.204	3779	3783	3785	rBV6	629	431	0.03%	0.004%
90	13.297	3809	3812	3816	rBV4	398	348	0.03%	0.004%
91	13.384	3837	3839	3843	rBV3	655	418	0.03%	0.004%
92	13.419	3847	3850	3851	rBV2	588	351	0.03%	0.004%
93	13.461	3855	3863	3866	rBV6	1677	2091	0.17%	0.021%
94	13.538	3881	3887	3889	rBV4	385	405	0.03%	0.004%
95	14.011	4032	4034	4036	rBV2	623	354	0.03%	0.004%
96	14.165	4079	4082	4087	rBV4	541	482	0.04%	0.005%
97	14.484	4179	4181	4186	rVB3	728	558	0.04%	0.006%
98	14.551	4200	4202	4206	rVB2	556	317	0.03%	0.003%
99	14.574	4206	4209	4213	rBV6	861	753	0.06%	0.008%
100	14.651	4230	4233	4237	rVB5	853	559	0.04%	0.006%




Sum of corrected areas: 9740098

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033570.D
Acq On : 10 Jan 2024 19:06
Operator : SY/MD
Sample : P1061-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

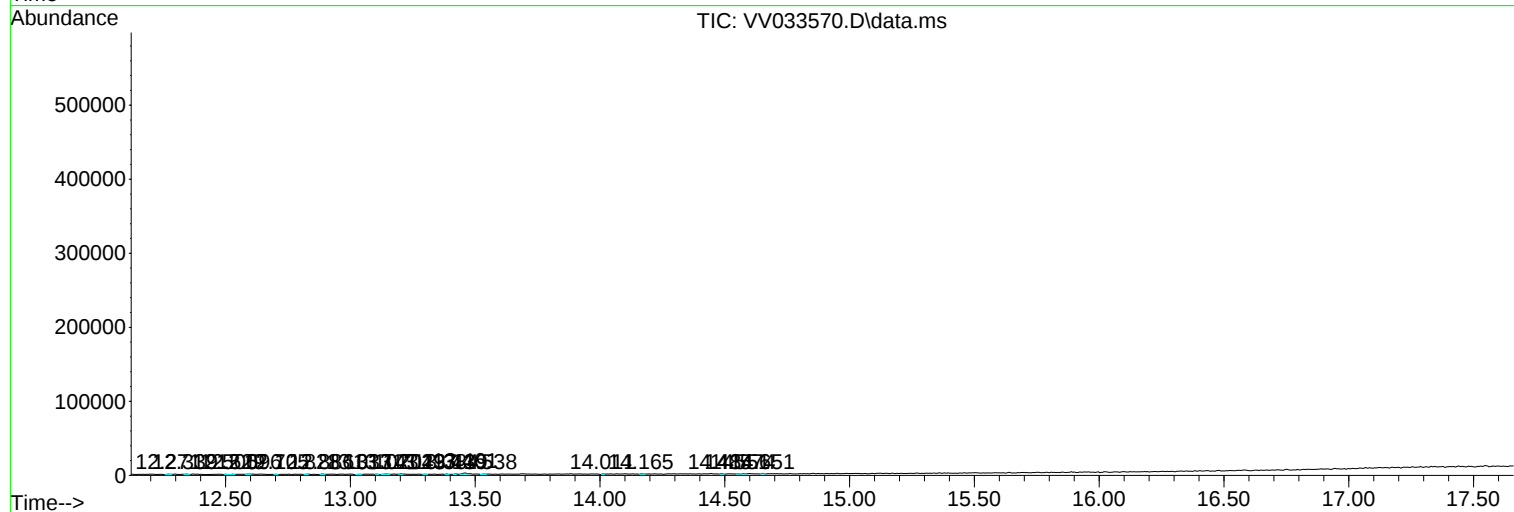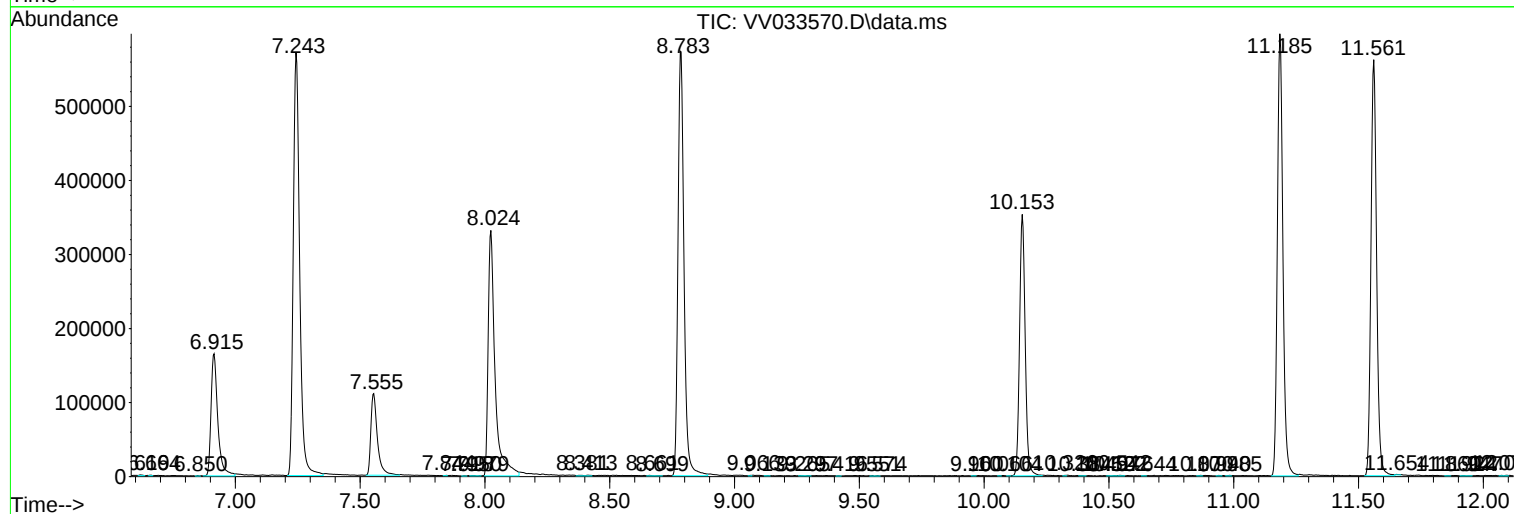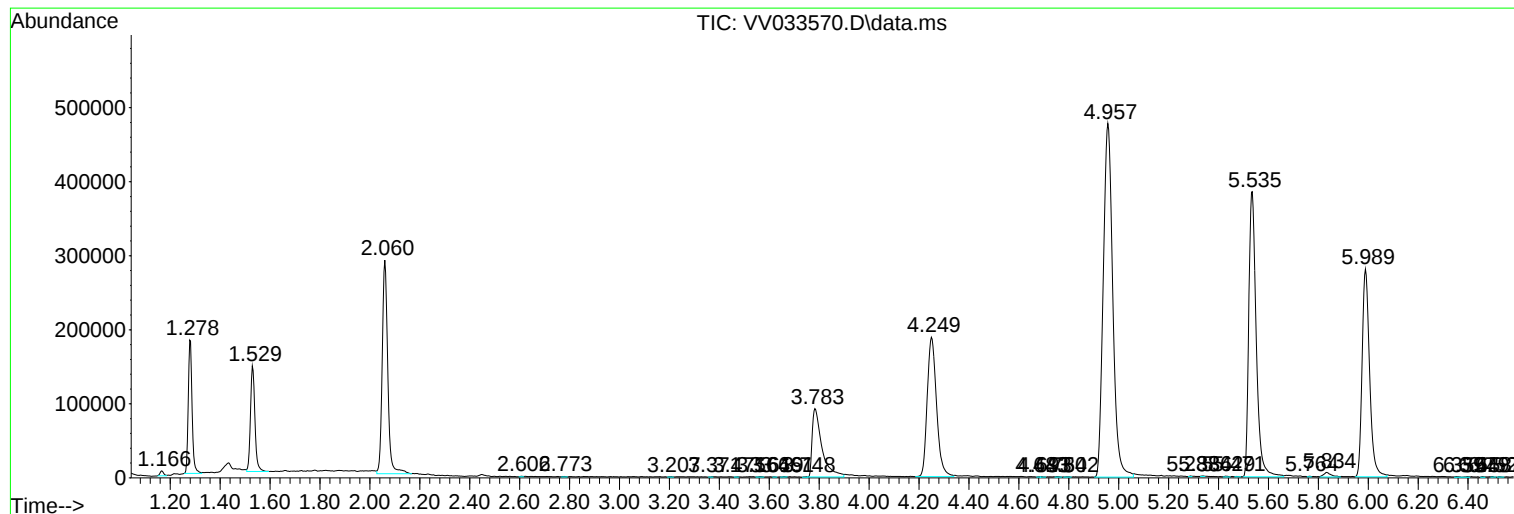

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033570.D
Acq On : 10 Jan 2024 19:06
Operator : SY/MD
Sample : P1061-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033570.D
Acq On : 10 Jan 2024 19:06
Operator : SY/MD
Sample : P1061-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------