

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033573.D
 Acq On : 10 Jan 2024 20:17
 Operator : SY/MD
 Sample : VIBLK262
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	34	39	44	rBV	3671	3327	0.28%	0.037%
2	1.217	50	55	57	rBV2	2400	2287	0.20%	0.025%
3	1.278	67	74	91	rBV	151720	161181	13.78%	1.792%
4	1.529	145	152	167	rVB	125393	151322	12.94%	1.682%
5	2.060	308	317	349	rVB	232409	364535	31.16%	4.053%
6	2.445	430	437	450	rVB2	5465	9888	0.85%	0.110%
7	2.561	461	473	484	rVB	4195	7512	0.64%	0.084%
8	2.748	529	531	536	rBV3	476	351	0.03%	0.004%
9	3.111	640	644	647	rBV4	341	314	0.03%	0.003%
10	3.166	658	661	664	rBV2	446	348	0.03%	0.004%
11	3.223	676	679	681	rBV3	569	330	0.03%	0.004%
12	3.587	790	792	798	rVB5	344	329	0.03%	0.004%
13	3.783	844	853	898	rBV	95697	267313	22.85%	2.972%
14	4.249	982	998	1025	rBV	174058	451483	38.59%	5.019%
15	4.461	1062	1064	1068	rBV2	464	364	0.03%	0.004%
16	4.481	1068	1070	1075	rVB5	452	335	0.03%	0.004%
17	4.580	1097	1101	1110	rVB6	1085	1461	0.12%	0.016%
18	4.751	1151	1154	1161	rBV5	512	518	0.04%	0.006%
19	4.786	1161	1165	1172	rBV6	515	754	0.06%	0.008%
20	4.841	1179	1182	1187	rVB4	591	524	0.04%	0.006%
21	4.870	1187	1191	1195	rBV3	638	588	0.05%	0.007%
22	4.957	1201	1218	1250	rBV2	435065	1169852	100.00%	13.006%
23	5.400	1352	1356	1358	rBV3	587	412	0.04%	0.005%
24	5.535	1386	1398	1427	rBV	332285	687583	58.78%	7.644%
25	5.693	1445	1447	1451	rBV4	646	430	0.04%	0.005%
26	5.834	1481	1491	1505	rVB6	6429	14750	1.26%	0.164%
27	5.915	1512	1516	1518	rBV5	364	291	0.02%	0.003%
28	5.989	1522	1539	1566	rBV	262492	550951	47.10%	6.125%
29	6.268	1624	1626	1630	rVB4	775	472	0.04%	0.005%
30	6.329	1643	1645	1649	rBV4	472	290	0.02%	0.003%
31	6.352	1649	1652	1656	rBV5	529	503	0.04%	0.006%
32	6.387	1660	1663	1665	rBV3	659	486	0.04%	0.005%
33	6.529	1703	1707	1711	rVB2	592	585	0.05%	0.007%
34	6.583	1720	1724	1725	rBV2	520	306	0.03%	0.003%
35	6.915	1815	1827	1856	rBV	152050	294146	25.14%	3.270%
36	7.133	1891	1895	1896	rBV2	498	334	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033573.D
 Acq On : 10 Jan 2024 20:17
 Operator : SY/MD
 Sample : VIBLK262
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	7.146	1897	1899	1902	rVV3	536	377	0.03%	0.004%
38	7.243	1918	1929	1963	rBV	487881	869766	74.35%	9.669%
39	7.555	2014	2026	2049	rBV	106445	193512	16.54%	2.151%
40	7.850	2115	2118	2120	rBV2	692	534	0.05%	0.006%
41	7.873	2122	2125	2128	rBV4	594	371	0.03%	0.004%
42	7.921	2137	2140	2147	rVB5	1067	775	0.07%	0.009%
43	7.979	2153	2158	2160	rBV3	376	351	0.03%	0.004%
44	8.024	2163	2172	2215	rBV	327036	635345	54.31%	7.063%
45	8.413	2290	2293	2297	rVB5	503	385	0.03%	0.004%
46	8.503	2319	2321	2325	rBV3	382	322	0.03%	0.004%
47	8.603	2349	2352	2355	rBV5	592	414	0.04%	0.005%
48	8.786	2396	2409	2438	rBV	497822	834063	71.30%	9.273%
49	9.043	2485	2489	2492	rVB5	614	459	0.04%	0.005%
50	9.088	2499	2503	2505	rBV4	1273	1017	0.09%	0.011%
51	9.165	2525	2527	2532	rVB4	532	431	0.04%	0.005%
52	9.191	2532	2535	2536	rBV3	458	289	0.02%	0.003%
53	9.259	2553	2556	2559	rBV2	355	294	0.03%	0.003%
54	9.284	2562	2564	2569	rVB3	418	346	0.03%	0.004%
55	9.329	2573	2578	2580	rBV3	385	344	0.03%	0.004%
56	9.490	2618	2628	2629	rBV5	2062	2623	0.22%	0.029%
57	9.606	2661	2664	2667	rVV3	478	302	0.03%	0.003%
58	9.670	2682	2684	2688	rVB4	575	362	0.03%	0.004%
59	9.728	2698	2702	2704	rBV2	542	398	0.03%	0.004%
60	9.818	2724	2730	2733	rBV3	412	340	0.03%	0.004%
61	9.876	2739	2748	2756	rBV4	2603	4733	0.40%	0.053%
62	10.034	2794	2797	2799	rBV2	418	288	0.02%	0.003%
63	10.152	2821	2834	2862	rVV	338424	543149	46.43%	6.038%
64	10.326	2886	2888	2897	rVB5	463	366	0.03%	0.004%
65	10.361	2897	2899	2903	rVB4	598	398	0.03%	0.004%
66	10.394	2903	2909	2911	rBV3	479	484	0.04%	0.005%
67	10.484	2926	2937	2944	rVV5	2627	4401	0.38%	0.049%
68	10.638	2983	2985	2990	rBV3	463	360	0.03%	0.004%
69	10.734	3011	3015	3019	rBV5	480	374	0.03%	0.004%
70	10.767	3019	3025	3029	rVB5	641	689	0.06%	0.008%
71	10.860	3046	3054	3063	rBV4	3693	6073	0.52%	0.068%
72	11.066	3114	3118	3121	rBV5	560	311	0.03%	0.003%
73	11.127	3130	3137	3145	rVV3	4873	7422	0.63%	0.083%
74	11.185	3145	3155	3178	rVV	493866	780554	66.72%	8.678%
75	11.561	3260	3272	3295	rBV	482282	770892	65.90%	8.570%
76	11.709	3316	3318	3324	rVB5	526	351	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033573.D
 Acq On : 10 Jan 2024 20:17
 Operator : SY/MD
 Sample : VIBLK262
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK262

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

77	11.799	3342	3346	3349	rBV5	516	354	0.03%	0.004%
78	11.844	3355	3360	3364	rBV3	522	449	0.04%	0.005%
79	11.886	3370	3373	3377	rVB4	555	373	0.03%	0.004%
80	11.914	3377	3382	3384	rBV3	362	318	0.03%	0.004%
81	12.117	3441	3445	3446	rBV2	544	295	0.03%	0.003%
82	12.191	3462	3468	3469	rBV3	463	308	0.03%	0.003%
83	12.374	3516	3525	3532	rBV3	1791	3048	0.26%	0.034%
84	12.467	3550	3554	3557	rBV4	699	473	0.04%	0.005%
85	12.586	3583	3591	3604	rVB3	7704	11588	0.99%	0.129%
86	12.734	3634	3637	3639	rBV2	710	508	0.04%	0.006%
87	13.004	3716	3721	3728	rBV8	499	821	0.07%	0.009%
88	13.204	3774	3783	3796	rVV2	16591	25466	2.18%	0.283%
89	13.320	3815	3819	3822	rVB4	461	329	0.03%	0.004%
90	13.445	3847	3858	3876	rBV	58431	100633	8.60%	1.119%
91	13.599	3901	3906	3909	rBV3	520	523	0.04%	0.006%
92	13.683	3924	3932	3947	rVV2	22221	33938	2.90%	0.377%
93	13.770	3954	3959	3962	rBV4	624	622	0.05%	0.007%
94	13.866	3985	3989	3993	rBV4	577	502	0.04%	0.006%
95	13.937	4006	4011	4012	rBV3	517	454	0.04%	0.005%
96	14.246	4104	4107	4108	rBV3	483	290	0.02%	0.003%
97	14.313	4125	4128	4131	rBV3	391	321	0.03%	0.004%
98	14.455	4164	4172	4178	rBV6	914	1575	0.13%	0.018%
99	14.557	4201	4204	4208	rBV2	511	457	0.04%	0.005%
100	15.133	4379	4383	4385	rBV4	722	636	0.05%	0.007%




Sum of corrected areas: 8995001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033573.D
Acq On : 10 Jan 2024 20:17
Operator : SY/MD
Sample : VIBLK262
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

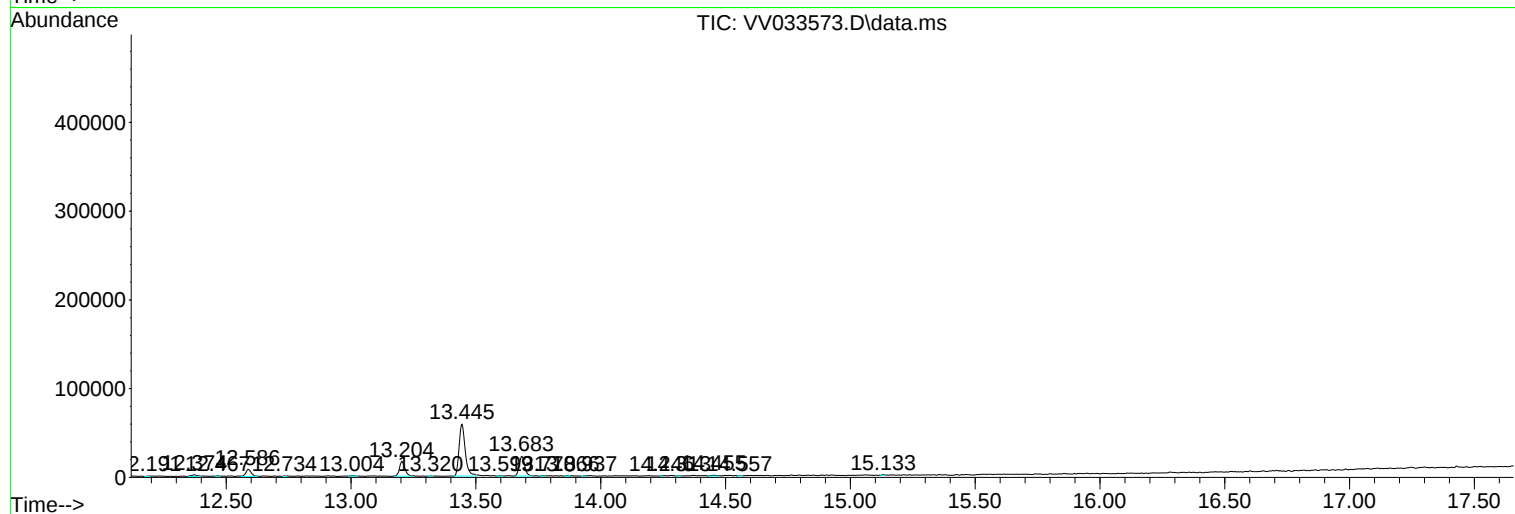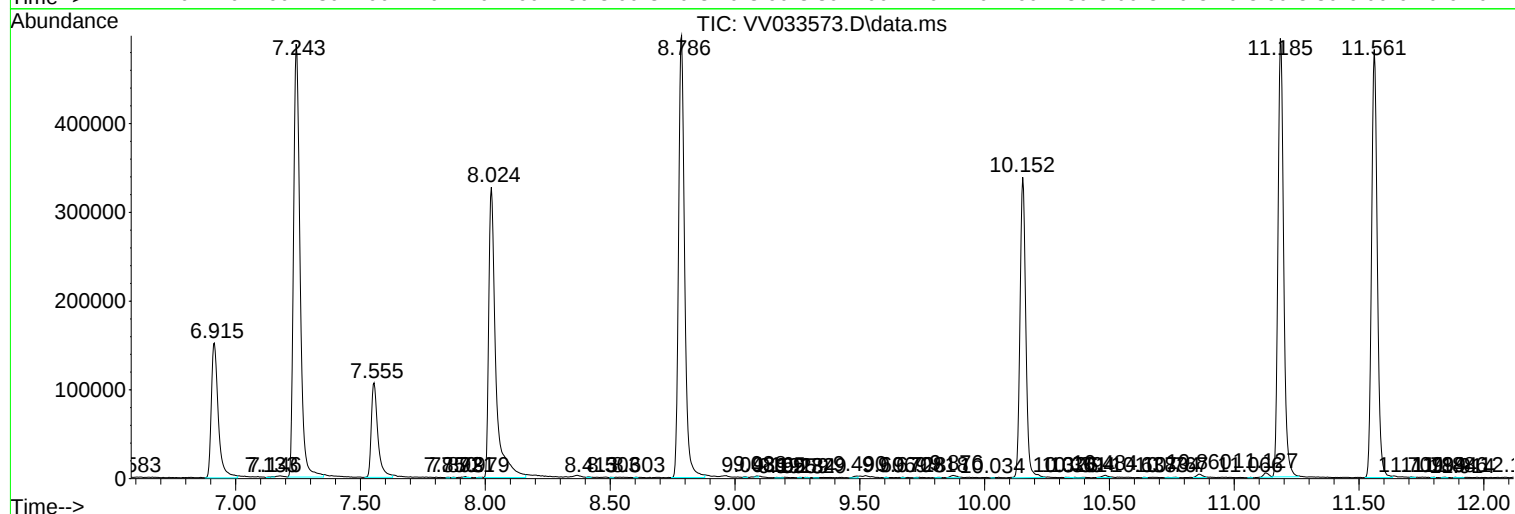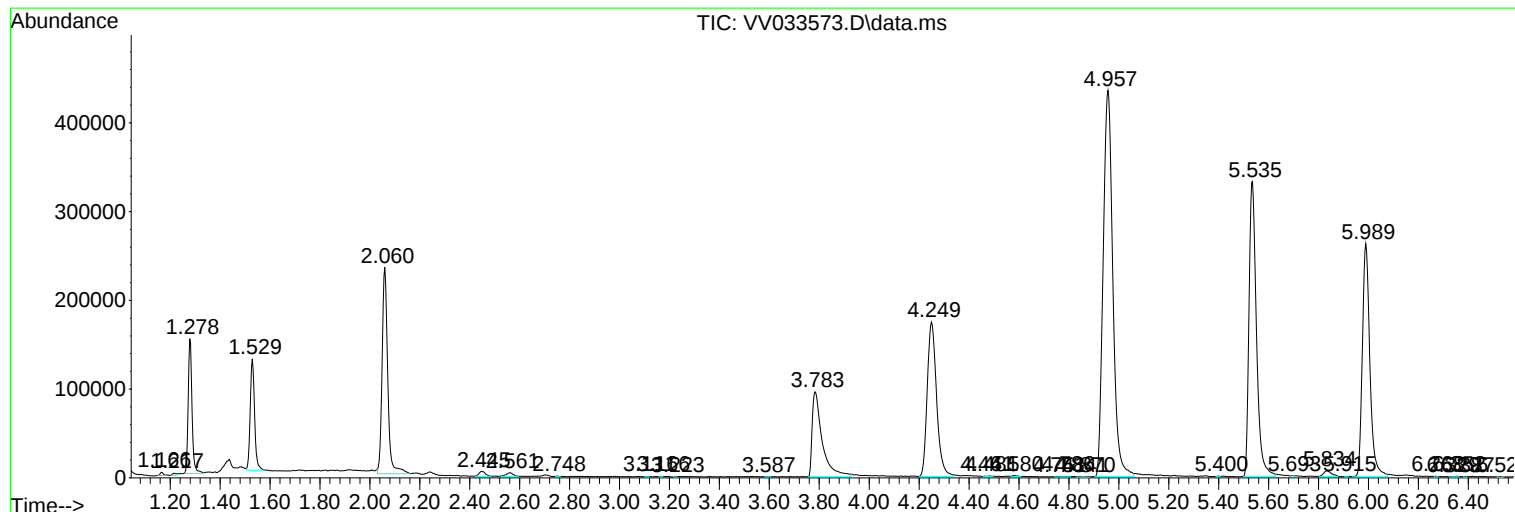

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033573.D
Acq On : 10 Jan 2024 20:17
Operator : SY/MD
Sample : VIBLK262
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033573.D
Acq On : 10 Jan 2024 20:17
Operator : SY/MD
Sample : VIBLK262
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
