

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033574.D
 Acq On : 10 Jan 2024 20:41
 Operator : SY/MD
 Sample : P1059-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

Signal : TIC: VV033574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rBV	194806	204049	15.29%	2.041%
2	1.529	145	152	169	rVB	150780	181732	13.61%	1.818%
3	2.060	308	317	336	rVB	297159	431786	32.34%	4.318%
4	3.204	670	673	674	rBV3	316	215	0.02%	0.002%
5	3.278	694	696	698	rBV2	384	119	0.01%	0.001%
6	3.783	844	853	887	rBV	96582	259601	19.45%	2.596%
7	4.249	983	998	1031	rBV	196106	504668	37.80%	5.047%
8	4.709	1139	1141	1142	rBV2	430	165	0.01%	0.002%
9	4.780	1158	1163	1166	rBV5	797	851	0.06%	0.009%
10	4.831	1174	1179	1180	rBV2	664	523	0.04%	0.005%
11	4.896	1196	1199	1201	rBV2	370	244	0.02%	0.002%
12	4.957	1201	1218	1254	rBV2	503678	1334961	100.00%	13.351%
13	5.532	1386	1397	1427	rBV	387428	794722	59.53%	7.948%
14	5.989	1526	1539	1567	rBV	290383	602594	45.14%	6.027%
15	6.442	1677	1680	1685	rVB4	550	436	0.03%	0.004%
16	6.465	1685	1687	1688	rBV2	536	196	0.01%	0.002%
17	6.542	1708	1711	1713	rBV	369	256	0.02%	0.003%
18	6.596	1726	1728	1731	rBV3	408	206	0.02%	0.002%
19	6.850	1804	1807	1808	rBV2	232	93	0.01%	0.001%
20	6.912	1814	1826	1849	rBV	167592	317354	23.77%	3.174%
21	7.243	1918	1929	1964	rBV	595737	1060634	79.45%	10.608%
22	7.555	2016	2026	2054	rBV	114668	214099	16.04%	2.141%
23	7.960	2150	2152	2153	rBV	229	95	0.01%	0.001%
24	7.979	2157	2158	2162	rVB2	542	249	0.02%	0.002%
25	8.024	2162	2172	2207	rBV	337696	650767	48.75%	6.508%
26	8.500	2317	2320	2322	rVB3	493	256	0.02%	0.003%
27	8.603	2347	2352	2355	rVB4	592	575	0.04%	0.006%
28	8.625	2355	2359	2361	rBV2	602	400	0.03%	0.004%
29	8.648	2363	2366	2369	rBV3	604	315	0.02%	0.003%
30	8.664	2369	2371	2372	rBV3	324	125	0.01%	0.001%
31	8.719	2384	2388	2392	rVB4	745	646	0.05%	0.006%
32	8.741	2392	2395	2397	rBV2	353	249	0.02%	0.002%
33	8.783	2397	2408	2444	rBV	581123	970141	72.67%	9.702%
34	9.075	2496	2499	2500	rBV3	548	320	0.02%	0.003%
35	9.204	2537	2539	2540	rBV3	236	134	0.01%	0.001%
36	9.265	2555	2558	2560	rBV3	598	358	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
 Data File : VV033574.D
 Acq On : 10 Jan 2024 20:41
 Operator : SY/MD
 Sample : P1059-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Title : VOC Analysis

37	9.374	2588	2592	2595	rBV3	405	342	0.03%	0.003%
38	9.391	2595	2597	2600	rVV3	405	267	0.02%	0.003%
39	9.452	2613	2616	2618	rBV	407	304	0.02%	0.003%
40	9.490	2622	2628	2630	rBV3	762	825	0.06%	0.008%
41	9.519	2635	2637	2640	rBV	524	394	0.03%	0.004%
42	9.628	2669	2671	2673	rBV	368	200	0.01%	0.002%
43	9.702	2691	2694	2699	rVB3	439	394	0.03%	0.004%
44	9.731	2699	2703	2705	rBV4	648	439	0.03%	0.004%
45	9.747	2706	2708	2711	rBV2	324	167	0.01%	0.002%
46	9.847	2737	2739	2740	rBV	366	183	0.01%	0.002%
47	9.924	2761	2763	2767	rBV3	412	184	0.01%	0.002%
48	10.024	2791	2794	2798	rBV4	382	335	0.03%	0.003%
49	10.095	2813	2816	2817	rBV2	333	189	0.01%	0.002%
50	10.153	2823	2834	2862	rVB	355884	567308	42.50%	5.674%
51	10.413	2912	2915	2919	rBV2	480	452	0.03%	0.005%
52	10.487	2932	2938	2941	rBV3	890	1009	0.08%	0.010%
53	10.519	2945	2948	2951	rBV4	595	502	0.04%	0.005%
54	10.725	3010	3012	3014	rBV2	482	176	0.01%	0.002%
55	10.754	3019	3021	3023	rBV2	391	247	0.02%	0.002%
56	10.960	3083	3085	3087	rBV2	323	205	0.02%	0.002%
57	11.072	3118	3120	3128	rBV4	596	594	0.04%	0.006%
58	11.127	3128	3137	3140	rBV8	1622	1942	0.15%	0.019%
59	11.185	3144	3155	3182	rBV	587415	926595	69.41%	9.267%
60	11.561	3260	3272	3293	rBV	579767	918365	68.79%	9.185%
61	12.062	3426	3428	3430	rBV3	304	144	0.01%	0.001%
62	12.140	3450	3452	3454	rVB2	374	162	0.01%	0.002%
63	12.159	3456	3458	3460	rBV3	334	139	0.01%	0.001%
64	12.480	3557	3558	3559	rBV	515	178	0.01%	0.002%
65	12.661	3609	3614	3617	rBV4	496	507	0.04%	0.005%
66	12.773	3647	3649	3650	rBV	317	102	0.01%	0.001%
67	12.812	3659	3661	3666	rBV3	558	414	0.03%	0.004%
68	13.210	3776	3785	3793	rBV4	3911	6143	0.46%	0.061%
69	13.448	3851	3859	3870	rBV	15434	26247	1.97%	0.262%
70	13.686	3926	3933	3943	rVB6	5591	8369	0.63%	0.084%
71	14.091	4057	4059	4062	rBV3	551	360	0.03%	0.004%
72	14.638	4227	4229	4231	rBV3	660	370	0.03%	0.004%




Sum of corrected areas: 9998887

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033574.D
Acq On : 10 Jan 2024 20:41
Operator : SY/MD
Sample : P1059-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

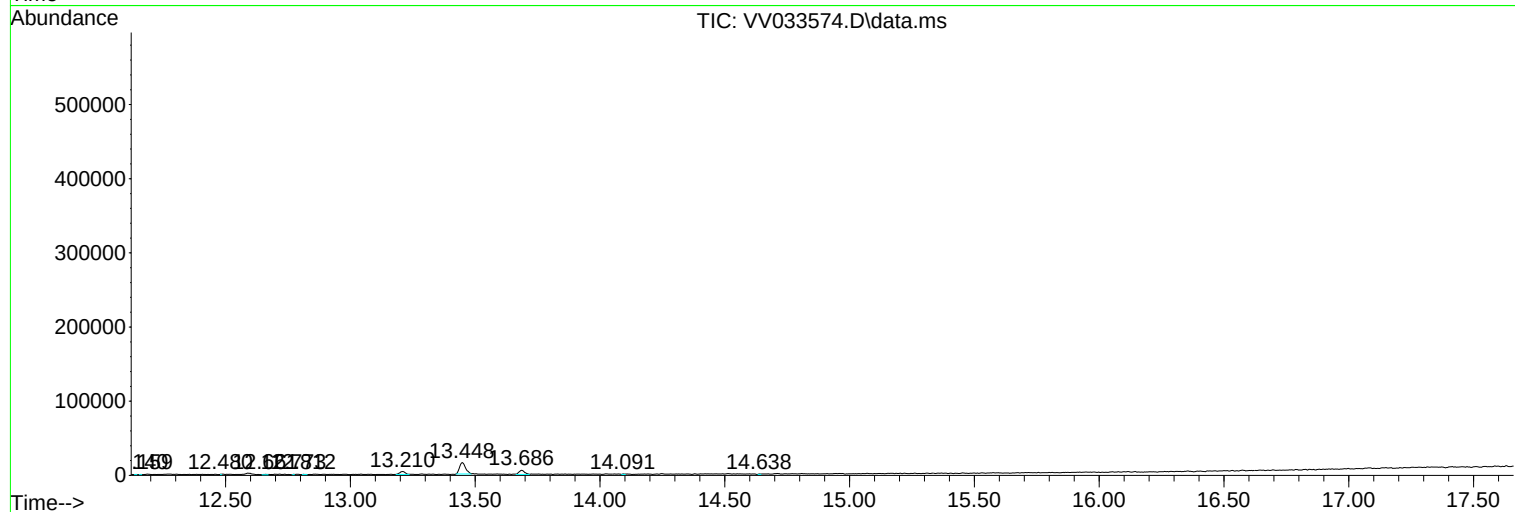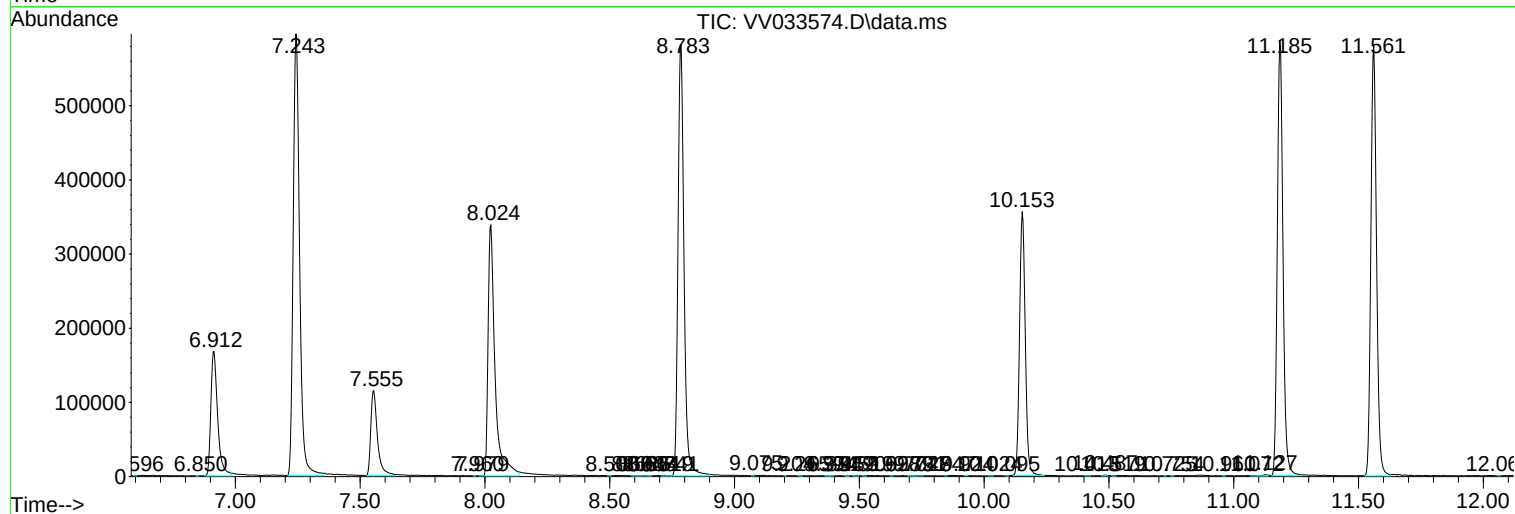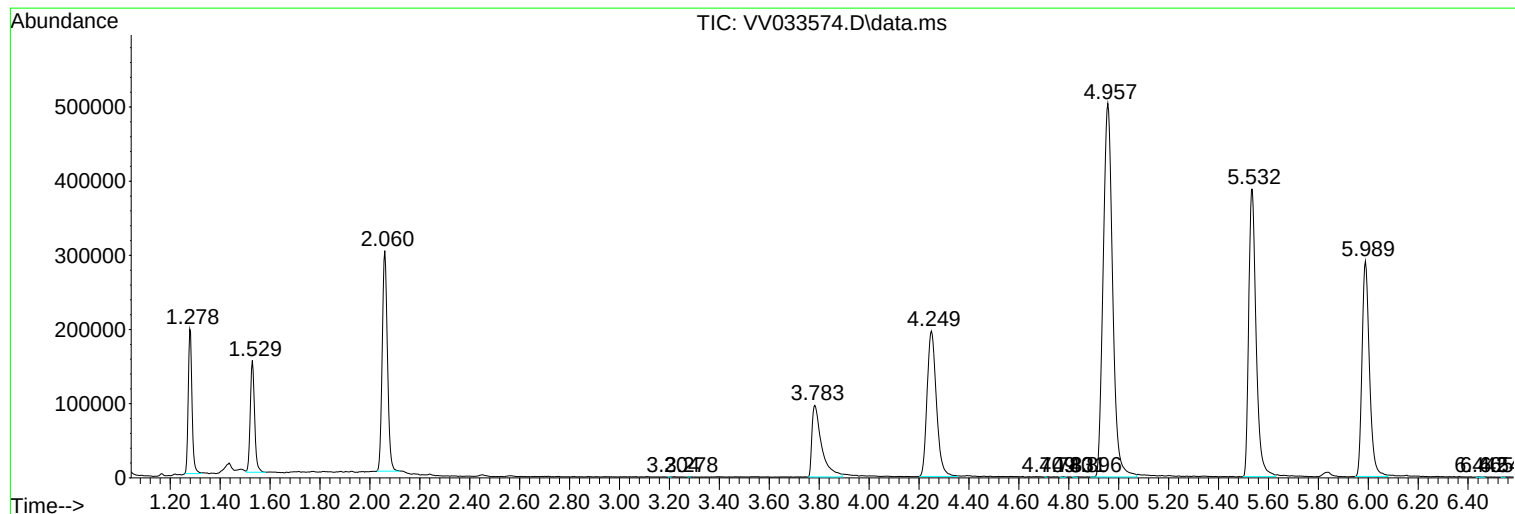

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033574.D
Acq On : 10 Jan 2024 20:41
Operator : SY/MD
Sample : P1059-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033574.D
Acq On : 10 Jan 2024 20:41
Operator : SY/MD
Sample : P1059-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc