


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011024\
Data File : VV033554.D
Acq On : 10 Jan 2024 11:28
Operator : SY/MD
Sample : BFB252
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB252

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis
Last Update : Thu Jan 11 00:32:34 2024

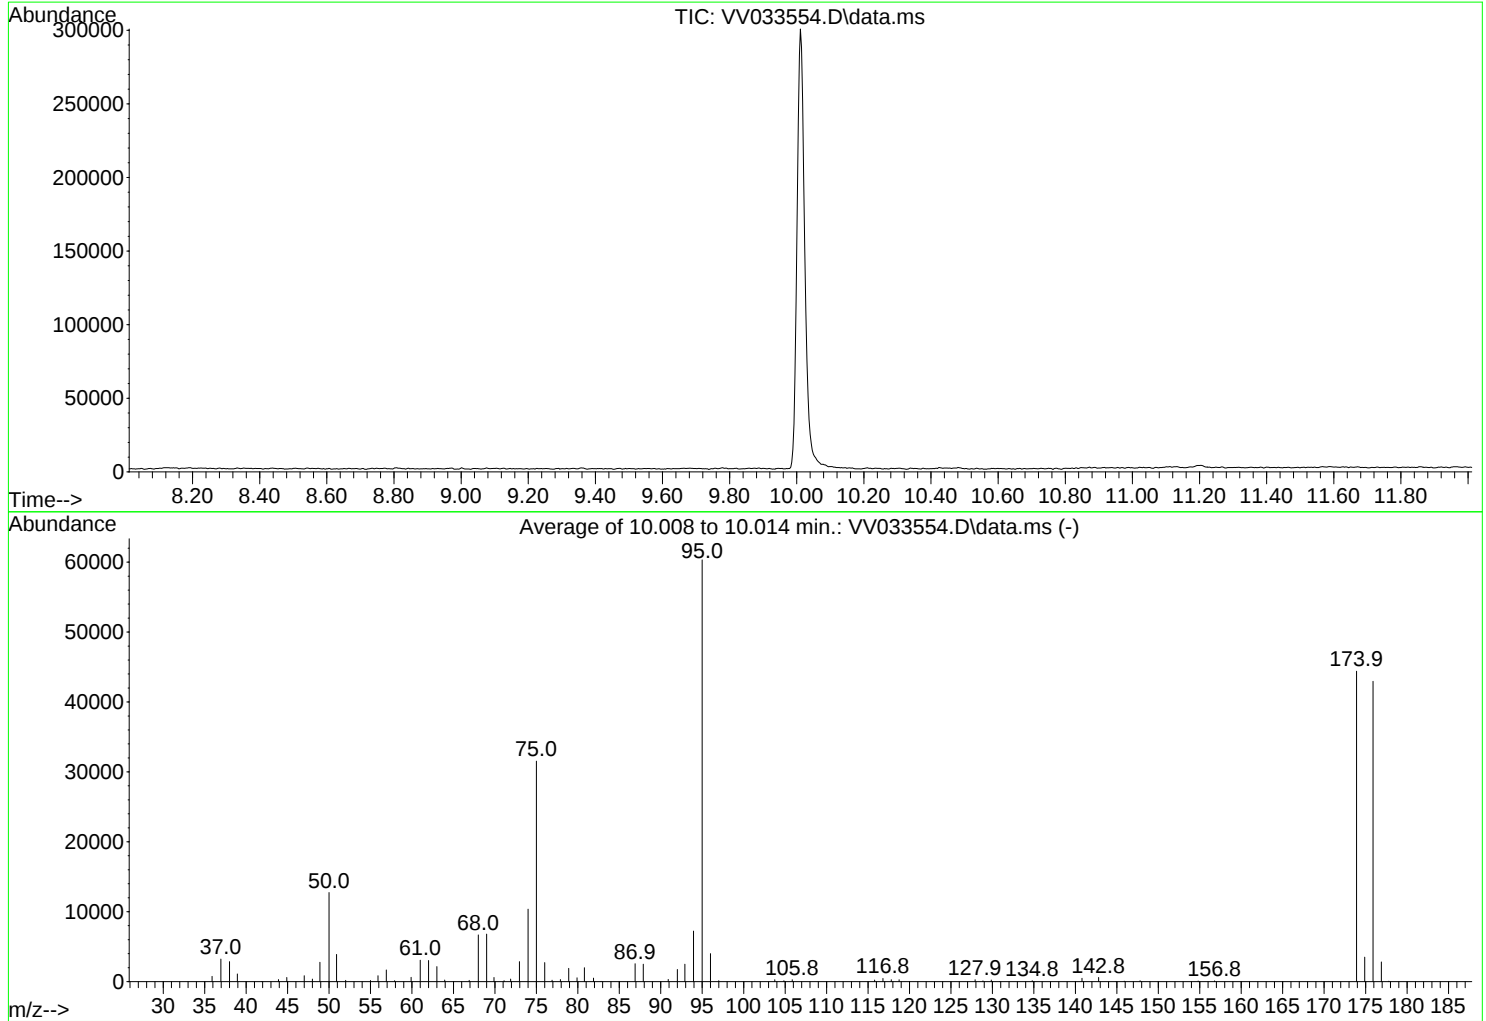

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	12749	PASS
75	95	30	80	52.3	31547	PASS
95	95	100	100	100.0	60328	PASS
96	95	5	9	6.7	4012	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	44389	PASS
175	174	5	9	7.9	3498	PASS
176	174	95	105	96.8	42952	PASS
177	176	5	10	6.6	2822	PASS

m/z	Abundance
38.90	166.0
39.90	256.0
40.90	286.0
41.90	139.0
42.90	278.0
43.90	426.0
55.00	219.0
56.10	114.0
56.80	132.0
67.00	102.0
76.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
35.90	767.0
37.00	3242.0
38.00	2884.0
39.00	1204.0
39.90	192.0
40.90	235.0
42.00	164.0
43.00	243.0
43.90	691.0
44.90	547.0
47.00	872.0
48.00	394.0
48.90	2760.0
50.00	12886.0
50.90	3792.0
52.00	188.0
55.00	396.0
55.90	942.0
57.00	1780.0
57.90	155.0
59.90	649.0
61.00	2985.0
62.00	3094.0
63.00	2079.0
64.00	204.0
66.90	299.0
68.00	6480.0
69.00	6802.0
69.90	638.0
71.00	127.0
71.90	341.0
73.00	2868.0
74.00	10106.0
75.00	31392.0
76.00	2698.0
76.90	391.0
77.90	305.0
78.90	1881.0
79.90	591.0
80.80	1962.0
81.90	506.0
86.90	2456.0
87.90	2264.0
90.90	296.0
92.00	1645.0
92.90	2397.0
94.00	7058.0
95.00	59032.0
96.00	3876.0
97.00	147.0
103.70	280.0
104.80	143.0
105.80	233.0
115.80	231.0
116.80	461.0
117.80	226.0
118.80	287.0
127.90	206.0
128.80	105.0
129.90	182.0
134.80	144.0
140.80	470.0
142.80	574.0
147.90	104.0
156.80	142.0
173.90	42696.0
174.90	3464.0
175.90	40768.0
176.90	2752.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
35.90	790.0
37.00	3350.0
38.00	2988.0
39.00	1298.0
39.90	204.0
41.00	251.0
41.90	166.0
43.00	286.0
43.90	733.0
44.90	622.0
47.00	895.0
48.00	373.0
48.90	2915.0
50.00	13173.0
50.90	4029.0
52.00	189.0
55.00	377.0
55.90	991.0
56.90	1863.0
57.90	135.0
59.90	648.0
61.00	3195.0
62.00	3094.0
63.00	2213.0
64.00	231.0
66.90	304.0
68.00	6961.0
69.00	6952.0
69.90	640.0
71.10	128.0
71.90	358.0
72.90	2960.0
74.00	10669.0
75.00	32480.0
76.00	2818.0
76.90	359.0
77.90	303.0
78.90	1953.0
79.90	557.0
80.80	2092.0
81.90	531.0
86.90	2692.0
87.90	2577.0
90.90	328.0
92.00	1787.0
92.90	2585.0
94.00	7468.0
95.00	62352.0
96.00	4104.0
97.00	138.0
103.70	282.0
104.80	149.0
105.90	275.0
115.80	238.0
116.80	475.0
117.80	299.0
118.70	275.0
127.90	290.0
128.80	117.0
129.80	239.0
134.80	149.0
140.80	504.0
142.80	636.0
144.90	105.0
145.90	113.0
147.80	139.0
154.80	139.0
156.80	121.0
173.90	45968.0
174.90	3649.0
175.90	44544.0
176.90	2934.0
177.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252

m/z	Abundance
35.90	729.0
36.90	3065.0
38.00	2731.0
39.00	1286.0
39.90	200.0
41.00	297.0
41.90	167.0
43.00	294.0
43.90	725.0
44.90	608.0
47.00	805.0
48.00	338.0
48.90	2630.0
50.00	12188.0
50.90	3823.0
52.00	171.0
55.00	345.0
55.90	980.0
56.90	1776.0
57.90	105.0
59.90	562.0
61.00	3037.0
62.00	2886.0
63.00	2159.0
63.90	253.0
66.90	280.0
68.00	6598.0
69.00	6606.0
69.90	515.0
71.20	140.0
71.90	385.0
72.90	2786.0
74.00	10310.0
75.00	30768.0
76.00	2671.0
76.90	308.0
77.90	257.0
78.90	1863.0
79.90	492.0
80.80	1955.0
81.90	483.0
82.80	107.0
86.90	2569.0
87.90	2615.0
90.90	319.0
92.00	1763.0
92.90	2517.0
93.90	7159.0
95.00	59600.0
96.00	4057.0
97.00	126.0
103.80	247.0
104.90	131.0
105.80	305.0
115.80	212.0
116.80	438.0
117.80	337.0
118.70	289.0
127.90	301.0
128.90	111.0
129.80	274.0
130.90	106.0
134.80	140.0
140.80	496.0
142.80	602.0
145.90	103.0
147.70	141.0
154.80	151.0
156.80	105.0
173.90	44504.0
174.90	3380.0
175.90	43544.0
176.90	2779.0
177.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB252