

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
 Data File : VV019967.D
 Acq On : 11 Jan 2021 15:31
 Operator : SY/MD
 Sample : VV0111WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV019967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	289962	295411	16.41%	2.164%
2	1.569	142	149	160	rBV	232251	261619	14.54%	1.917%
3	2.110	307	317	354	rVB	491226	758976	42.17%	5.561%
4	2.511	435	442	443	rBV5	2023	2270	0.13%	0.017%
5	3.064	611	614	615	rBV3	854	481	0.03%	0.004%
6	3.100	620	625	627	rBV3	588	467	0.03%	0.003%
7	3.142	635	638	643	rVB3	879	670	0.04%	0.005%
8	3.174	643	648	651	rBV4	886	999	0.06%	0.007%
9	3.251	670	672	678	rVB3	763	765	0.04%	0.006%
10	3.283	678	682	683	rBV3	614	438	0.02%	0.003%
11	3.335	693	698	701	rVB5	512	498	0.03%	0.004%
12	3.370	707	709	710	rBV	414	217	0.01%	0.002%
13	3.389	713	715	719	rVB3	685	406	0.02%	0.003%
14	3.409	719	721	723	rBV	437	277	0.02%	0.002%
15	3.518	753	755	759	rVB2	629	412	0.02%	0.003%
16	3.592	774	778	783	rBV4	723	670	0.04%	0.005%
17	3.621	783	787	788	rBV	774	407	0.02%	0.003%
18	3.650	792	796	801	rVV5	434	498	0.03%	0.004%
19	3.675	801	804	806	rBV3	450	352	0.02%	0.003%
20	3.701	810	812	816	rVB2	571	292	0.02%	0.002%
21	3.724	817	819	821	rBV	408	226	0.01%	0.002%
22	3.827	848	851	853	rBV3	645	434	0.02%	0.003%
23	3.843	853	856	859	rVB2	808	496	0.03%	0.004%
24	3.894	859	872	911	rBV2	123632	389361	21.63%	2.853%
25	4.354	998	1015	1042	rBV	297532	731847	40.66%	5.362%
26	4.627	1095	1100	1102	rBV4	775	683	0.04%	0.005%
27	4.672	1110	1114	1115	rBV3	1124	818	0.05%	0.006%
28	4.910	1186	1188	1190	rBV2	486	311	0.02%	0.002%
29	5.052	1213	1232	1260	rBV2	698293	1799808	100.00%	13.186%
30	5.408	1341	1343	1345	rBV3	627	249	0.01%	0.002%
31	5.621	1394	1409	1429	rBV	497304	986415	54.81%	7.227%
32	5.839	1474	1477	1479	rBV3	827	464	0.03%	0.003%
33	5.910	1488	1499	1518	rVB2	32651	69743	3.88%	0.511%
34	6.007	1526	1529	1533	rBV4	1127	981	0.05%	0.007%
35	6.074	1533	1550	1582	rVV2	404160	829287	46.08%	6.076%
36	6.286	1613	1616	1621	rVB5	889	620	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
 Data File : VV019967.D
 Acq On : 11 Jan 2021 15:31
 Operator : SY/MD
 Sample : VV0111WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.389	1645	1648	1650	rBV	613	396	0.02%	0.003%
38	6.470	1671	1673	1676	rVB2	631	285	0.02%	0.002%
39	6.511	1683	1686	1688	rBV	343	219	0.01%	0.002%
40	6.804	1774	1777	1780	rBV3	504	395	0.02%	0.003%
41	6.897	1804	1806	1809	rVB2	670	279	0.02%	0.002%
42	6.926	1812	1815	1818	rVB3	793	462	0.03%	0.003%
43	6.949	1818	1822	1823	rBV3	344	244	0.01%	0.002%
44	6.990	1823	1835	1855	rBV	228495	405480	22.53%	2.971%
45	7.177	1890	1893	1895	rBV3	1032	609	0.03%	0.004%
46	7.277	1921	1924	1925	rBV2	620	397	0.02%	0.003%
47	7.322	1926	1938	1969	rVV	804720	1396237	77.58%	10.229%
48	7.627	2022	2033	2056	rBV	156719	275921	15.33%	2.022%
49	7.945	2130	2132	2136	rVB3	466	275	0.02%	0.002%
50	7.984	2137	2144	2153	rVB10	2891	4947	0.27%	0.036%
51	8.055	2158	2166	2168	rBV4	636	811	0.05%	0.006%
52	8.093	2168	2178	2220	rBV2	407716	816689	45.38%	5.983%
53	8.733	2374	2377	2379	rBV2	660	460	0.03%	0.003%
54	8.785	2390	2393	2398	rBV4	653	608	0.03%	0.004%
55	8.858	2403	2416	2441	rBV	755200	1232939	68.50%	9.033%
56	9.093	2488	2489	2492	rBV2	850	421	0.02%	0.003%
57	9.293	2548	2551	2555	rBV3	389	317	0.02%	0.002%
58	9.366	2572	2574	2577	rBV3	473	319	0.02%	0.002%
59	9.383	2577	2579	2586	rVB3	617	427	0.02%	0.003%
60	9.453	2597	2601	2603	rBV3	374	315	0.02%	0.002%
61	9.489	2609	2612	2615	rBV3	708	526	0.03%	0.004%
62	9.694	2674	2676	2678	rBV2	424	250	0.01%	0.002%
63	9.775	2698	2701	2702	rBV2	516	227	0.01%	0.002%
64	9.887	2734	2736	2739	rVV2	785	402	0.02%	0.003%
65	9.910	2741	2743	2748	rVV4	898	681	0.04%	0.005%
66	9.942	2748	2753	2761	rVV4	1782	2072	0.12%	0.015%
67	9.990	2765	2768	2772	rBV3	494	419	0.02%	0.003%
68	10.013	2772	2775	2779	rVB2	552	499	0.03%	0.004%
69	10.045	2779	2785	2793	rBV5	748	1258	0.07%	0.009%
70	10.122	2807	2809	2812	rVB2	511	288	0.02%	0.002%
71	10.141	2812	2815	2818	rBV3	482	392	0.02%	0.003%
72	10.222	2828	2840	2860	rBV	489614	762319	42.36%	5.585%
73	10.350	2878	2880	2883	rBV4	566	290	0.02%	0.002%
74	10.553	2933	2943	2950	rBV7	1984	2684	0.15%	0.020%
75	10.582	2950	2952	2954	rBV3	538	290	0.02%	0.002%
76	10.624	2961	2965	2966	rBV2	581	371	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
 Data File : VV019967.D
 Acq On : 11 Jan 2021 15:31
 Operator : SY/MD
 Sample : VV0111WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >




Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
 Title : VOC Analysis

77	10.633	2966	2968	2972	rVB3	766	516	0.03%	0.004%
78	10.862	3034	3039	3044	rVB4	1054	1140	0.06%	0.008%
79	10.887	3044	3047	3049	rBV2	461	246	0.01%	0.002%
80	10.919	3051	3057	3065	rVV6	2250	3461	0.19%	0.025%
81	10.965	3069	3071	3075	rVB3	603	322	0.02%	0.002%
82	11.051	3096	3098	3103	rVB3	1171	760	0.04%	0.006%
83	11.083	3103	3108	3109	rBV	560	499	0.03%	0.004%
84	11.257	3150	3162	3188	rBV	796842	1239570	68.87%	9.082%
85	11.453	3219	3223	3225	rBV3	750	681	0.04%	0.005%
86	11.630	3266	3278	3303	rBV	837754	1322819	73.50%	9.692%
87	11.842	3341	3344	3349	rBB2	683	631	0.04%	0.005%
88	11.868	3349	3352	3354	rBV3	606	350	0.02%	0.003%
89	11.977	3383	3386	3387	rBV2	487	247	0.01%	0.002%
90	12.038	3403	3405	3408	rVB2	804	325	0.02%	0.002%
91	12.103	3421	3425	3427	rBV3	554	361	0.02%	0.003%
92	12.492	3542	3546	3551	rBV4	1031	867	0.05%	0.006%
93	12.656	3590	3597	3604	rBV9	5102	6892	0.38%	0.050%
94	13.276	3781	3790	3802	rVB8	5654	9228	0.51%	0.068%
95	13.517	3859	3865	3877	rVB3	5167	7647	0.42%	0.056%
96	13.617	3894	3896	3898	rBV	479	250	0.01%	0.002%
97	13.842	3960	3966	3968	rBV3	1026	814	0.05%	0.006%
98	13.923	3988	3991	3996	rBV3	726	595	0.03%	0.004%
99	14.109	4047	4049	4054	rVB4	672	311	0.02%	0.002%
100	14.151	4060	4062	4067	rBV4	646	326	0.02%	0.002%

Sum of corrected areas: 13649146

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

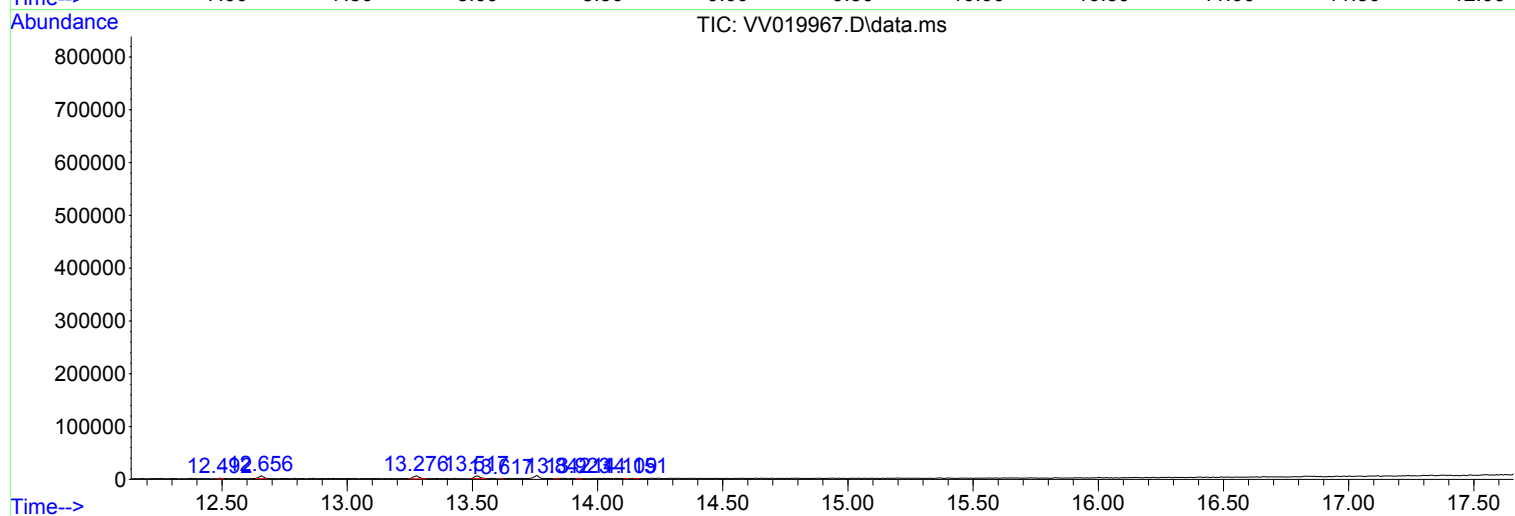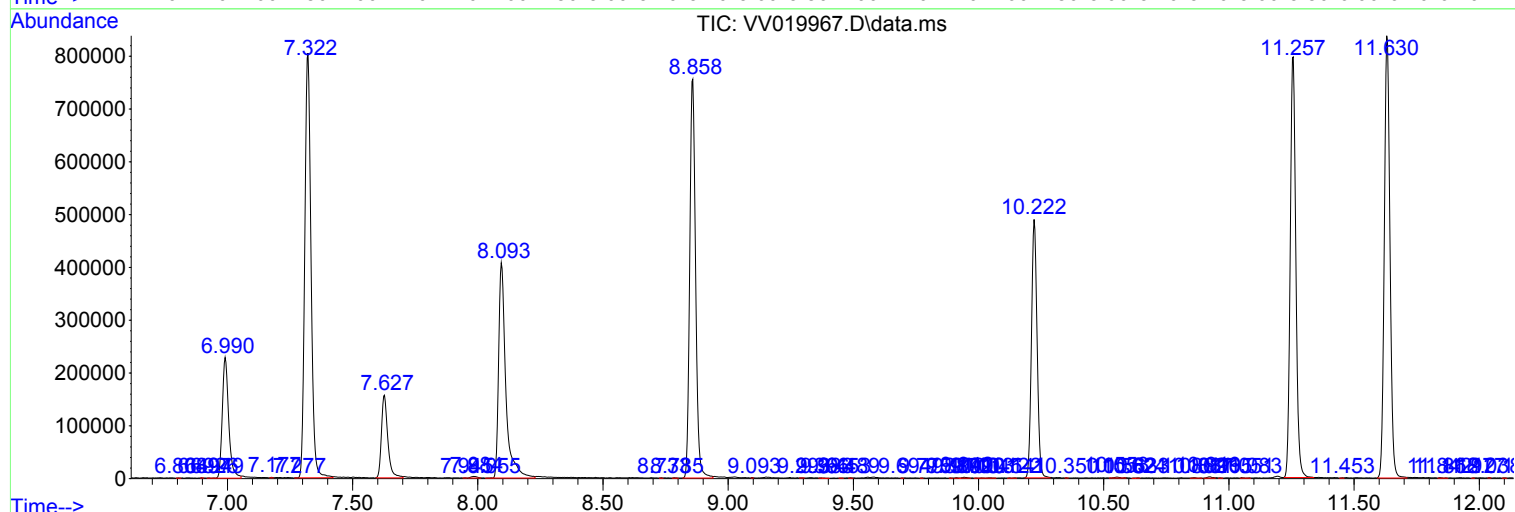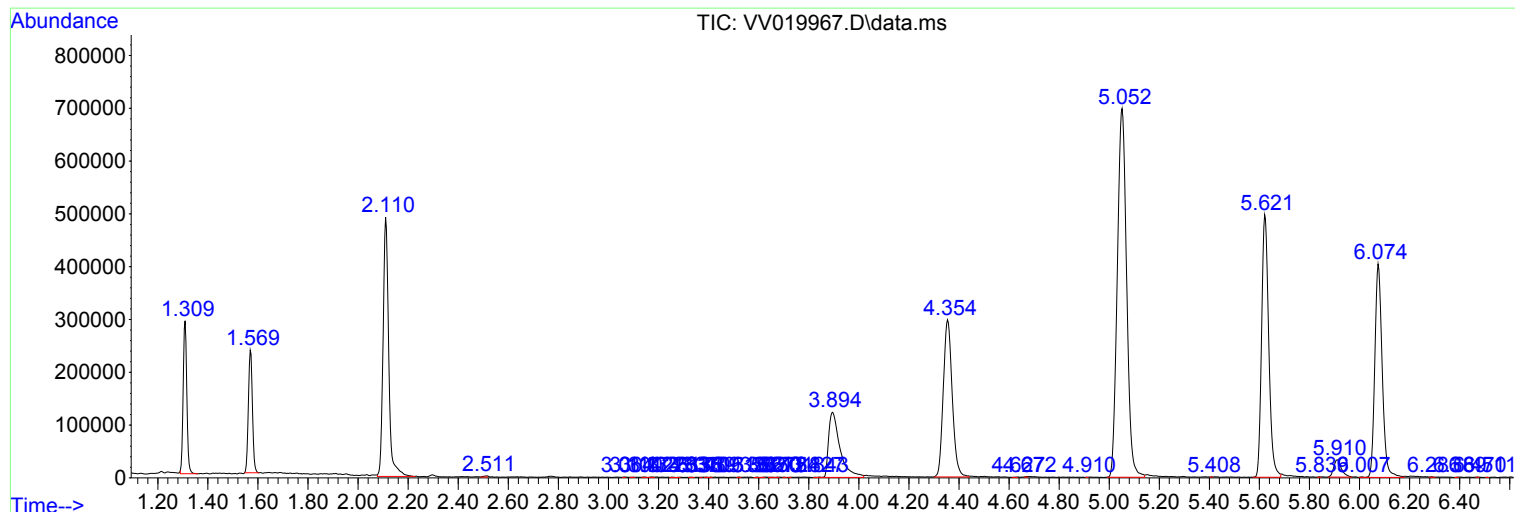

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
Data File : VV019967.D
Acq On : 11 Jan 2021 15:31
Operator : SY/MD
Sample : VV0111WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK71

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
Data File : VV019967.D
Acq On : 11 Jan 2021 15:31
Operator : SY/MD
Sample : VV0111WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK71

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
