

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
 Data File : VV019973.D
 Acq On : 11 Jan 2021 17:52
 Operator : SY/MD
 Sample : M1064-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV019973.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	78	rVB	266652	259097	15.36%	2.038%
2	1.569	142	149	164	rVB	212240	240324	14.25%	1.890%
3	2.109	308	317	348	rVB	436105	666199	39.49%	5.239%
4	2.328	383	385	391	rVB4	993	961	0.06%	0.008%
5	2.354	391	393	396	rBV2	655	389	0.02%	0.003%
6	2.601	467	470	473	rBV3	714	619	0.04%	0.005%
7	2.630	477	479	483	rVV4	1152	676	0.04%	0.005%
8	2.669	489	491	495	rBV3	692	470	0.03%	0.004%
9	2.688	495	497	502	rVV4	688	562	0.03%	0.004%
10	2.711	502	504	507	rVB	545	211	0.01%	0.002%
11	2.971	582	585	586	rBV2	418	253	0.01%	0.002%
12	3.119	629	631	633	rBV2	383	211	0.01%	0.002%
13	3.167	642	646	648	rBV4	462	358	0.02%	0.003%
14	3.296	680	686	688	rBV4	595	601	0.04%	0.005%
15	3.360	704	706	708	rBV	378	193	0.01%	0.002%
16	3.399	716	718	723	rVB4	665	431	0.03%	0.003%
17	3.495	746	748	750	rVB4	496	222	0.01%	0.002%
18	3.511	750	753	755	rBV2	235	142	0.01%	0.001%
19	3.547	759	764	767	rBV3	829	797	0.05%	0.006%
20	3.592	775	778	781	rBV2	527	327	0.02%	0.003%
21	3.608	781	783	784	rBV2	303	104	0.01%	0.001%
22	3.727	815	820	821	rBV2	609	325	0.02%	0.003%
23	3.769	832	833	834	rBV	292	77	0.00%	0.001%
24	3.788	837	839	840	rBV	431	173	0.01%	0.001%
25	3.833	848	853	855	rBV4	758	699	0.04%	0.005%
26	3.900	862	874	909	rBV	112316	366788	21.74%	2.885%
27	4.354	1001	1015	1041	rVB	280099	674686	39.99%	5.306%
28	4.701	1120	1123	1125	rBV2	571	297	0.02%	0.002%
29	4.775	1144	1146	1147	rBV	396	149	0.01%	0.001%
30	4.807	1154	1156	1158	rBV2	546	284	0.02%	0.002%
31	4.904	1184	1186	1189	rBV3	299	155	0.01%	0.001%
32	4.916	1189	1190	1191	rVV3	355	75	0.00%	0.001%
33	4.926	1191	1193	1196	rVV3	591	314	0.02%	0.002%
34	5.051	1213	1232	1261	rBV2	654665	1687020	100.00%	13.267%
35	5.466	1359	1361	1363	rBV2	355	177	0.01%	0.001%
36	5.556	1387	1389	1390	rBV	504	179	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011121\
 Data File : VW019973.D
 Acq On : 11 Jan 2021 17:52
 Operator : SY/MD
 Sample : M1064-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

37	5.621	1397	1409	1437	rBV	472068	951616	56.41%	7.484%
38	5.910	1490	1499	1518	rVB2	32654	67113	3.98%	0.528%
39	6.074	1537	1550	1584	rBV	377805	772740	45.81%	6.077%
40	6.389	1642	1648	1651	rBV7	1254	1576	0.09%	0.012%
41	6.582	1706	1708	1713	rBV3	640	529	0.03%	0.004%
42	6.740	1756	1757	1760	rVB2	841	364	0.02%	0.003%
43	6.759	1760	1763	1764	rBV2	890	406	0.02%	0.003%
44	6.830	1783	1785	1786	rBV	512	243	0.01%	0.002%
45	6.875	1797	1799	1800	rBV2	487	229	0.01%	0.002%
46	6.932	1815	1817	1819	rBV3	391	163	0.01%	0.001%
47	6.990	1823	1835	1856	rBV	204032	372705	22.09%	2.931%
48	7.321	1926	1938	1965	rBV	740733	1273528	75.49%	10.015%
49	7.627	2023	2033	2052	rBV	143186	247283	14.66%	1.945%
50	7.984	2133	2144	2154	rBV8	2917	6185	0.37%	0.049%
51	8.032	2157	2159	2162	rVV3	459	238	0.01%	0.002%
52	8.093	2167	2178	2220	rBV2	387010	778007	46.12%	6.118%
53	8.440	2282	2286	2289	rBV	913	859	0.05%	0.007%
54	8.588	2330	2332	2335	rBV	459	275	0.02%	0.002%
55	8.685	2360	2362	2365	rBV2	709	479	0.03%	0.004%
56	8.858	2404	2416	2441	rBV	722013	1183666	70.16%	9.309%
57	9.501	2614	2616	2620	rBV3	470	207	0.01%	0.002%
58	9.524	2620	2623	2625	rBV4	776	414	0.02%	0.003%
59	9.585	2639	2642	2644	rBV3	689	462	0.03%	0.004%
60	9.710	2678	2681	2684	rBV2	616	512	0.03%	0.004%
61	9.762	2695	2697	2704	rBV3	500	502	0.03%	0.004%
62	9.791	2704	2706	2710	rBV3	741	393	0.02%	0.003%
63	9.842	2720	2722	2724	rVB2	547	227	0.01%	0.002%
64	9.868	2724	2730	2733	rBV3	1221	1246	0.07%	0.010%
65	9.910	2739	2743	2744	rBV3	472	315	0.02%	0.002%
66	10.080	2794	2796	2798	rBV3	675	291	0.02%	0.002%
67	10.173	2823	2825	2828	rBV2	669	338	0.02%	0.003%
68	10.222	2828	2840	2861	rVV	465710	724812	42.96%	5.700%
69	10.405	2893	2897	2900	rBV3	628	500	0.03%	0.004%
70	10.447	2908	2910	2911	rBV	598	272	0.02%	0.002%
71	10.543	2937	2940	2941	rBV	674	357	0.02%	0.003%
72	10.588	2951	2954	2956	rBV2	745	478	0.03%	0.004%
73	10.601	2956	2958	2961	rVB	542	245	0.01%	0.002%
74	10.672	2977	2980	2982	rBV2	624	446	0.03%	0.004%
75	10.714	2991	2993	2996	rBV3	721	470	0.03%	0.004%
76	10.768	3008	3010	3012	rVB	542	222	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
 Data File : VV019973.D
 Acq On : 11 Jan 2021 17:52
 Operator : SY/MD
 Sample : M1064-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.781	3012	3014	3018	rBV3	545	462	0.03%	0.004%
78	10.852	3033	3036	3037	rBV2	570	240	0.01%	0.002%
79	10.929	3055	3060	3061	rBV2	932	749	0.04%	0.006%
80	10.987	3076	3078	3082	rBV3	531	407	0.02%	0.003%
81	11.045	3095	3096	3098	rBV	536	209	0.01%	0.002%
82	11.119	3117	3119	3122	rVB2	439	207	0.01%	0.002%
83	11.135	3122	3124	3126	rBV	438	164	0.01%	0.001%
84	11.148	3126	3128	3131	rBV3	640	443	0.03%	0.003%
85	11.196	3137	3143	3145	rBV3	1450	1411	0.08%	0.011%
86	11.257	3150	3162	3186	rBV	755056	1183524	70.15%	9.307%
87	11.630	3266	3278	3296	rBV	779218	1227632	72.77%	9.654%
88	12.276	3476	3479	3482	rVB3	565	295	0.02%	0.002%
89	12.659	3592	3598	3605	rBV7	1687	2254	0.13%	0.018%
90	12.778	3633	3635	3637	rBV	422	217	0.01%	0.002%
91	12.874	3662	3665	3666	rBV	658	329	0.02%	0.003%
92	13.013	3706	3708	3710	rBV2	499	312	0.02%	0.002%
93	13.611	3889	3894	3900	rBV6	842	1070	0.06%	0.008%
94	14.099	4043	4046	4047	rBV2	792	433	0.03%	0.003%




Sum of corrected areas: 12715816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
Data File : VV019973.D
Acq On : 11 Jan 2021 17:52
Operator : SY/MD
Sample : M1064-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

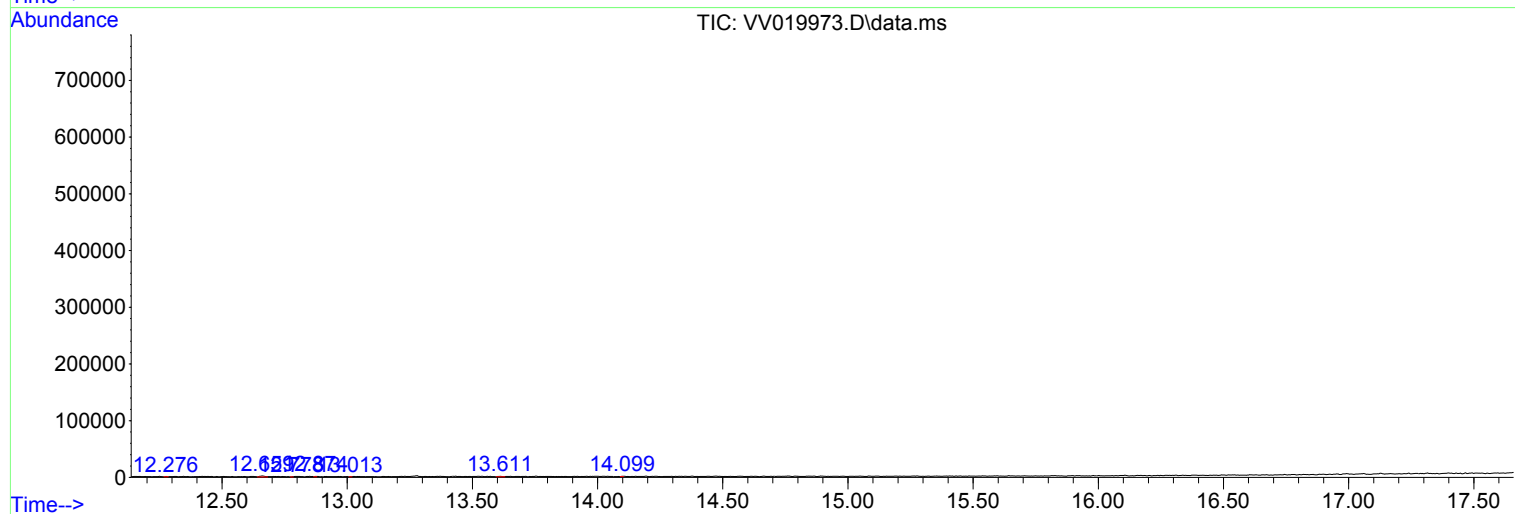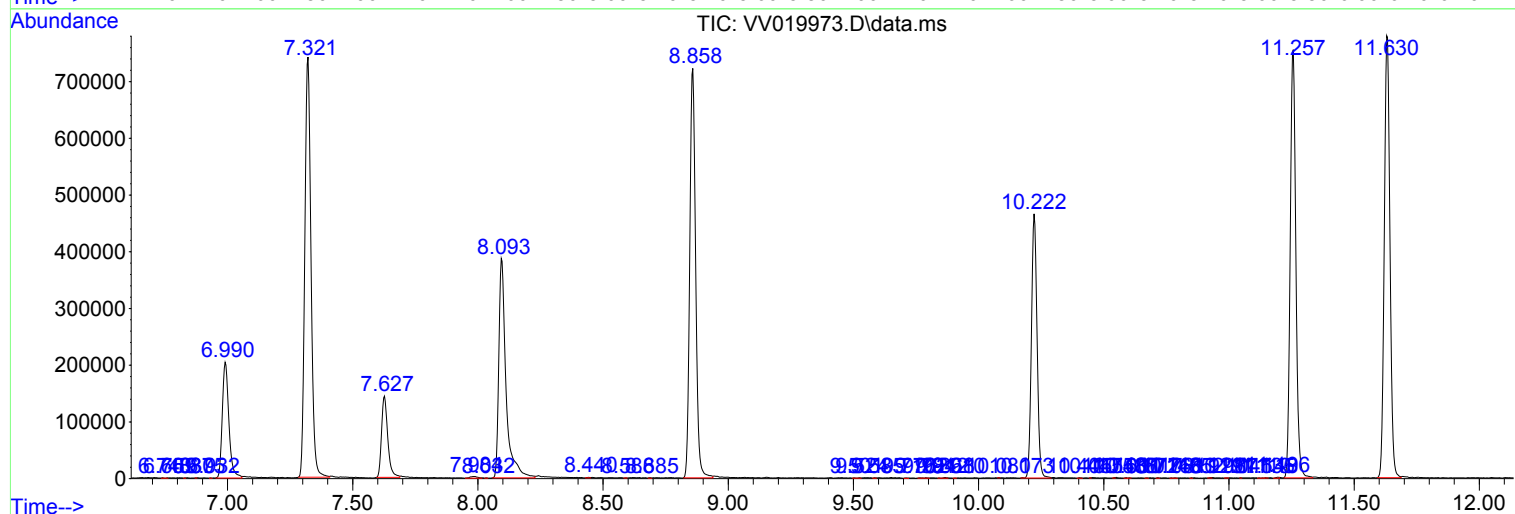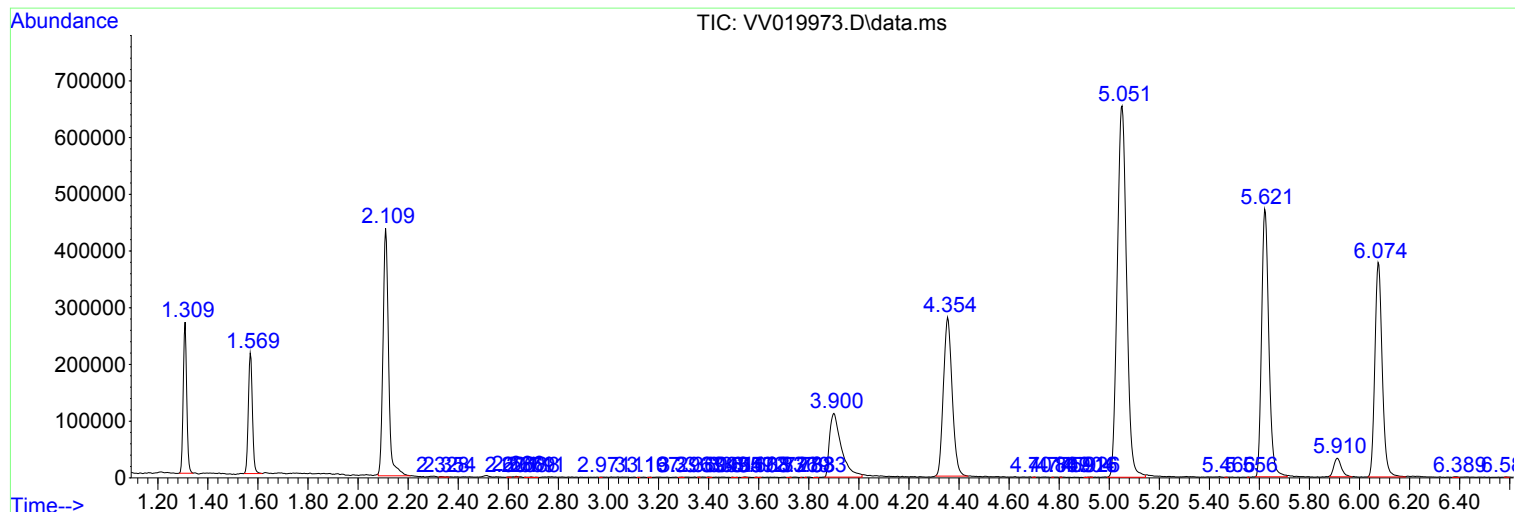

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
Data File : VV019973.D
Acq On : 11 Jan 2021 17:52
Operator : SY/MD
Sample : M1064-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
Data File : VV019973.D
Acq On : 11 Jan 2021 17:52
Operator : SY/MD
Sample : M1064-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
