


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011121\
Data File : VV019958.D
Acq On : 11 Jan 2021 09:31
Operator : SY/MD
Sample : BFB78
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB78

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Title : VOC Analysis
Last Update : Mon Jan 11 13:51:52 2021

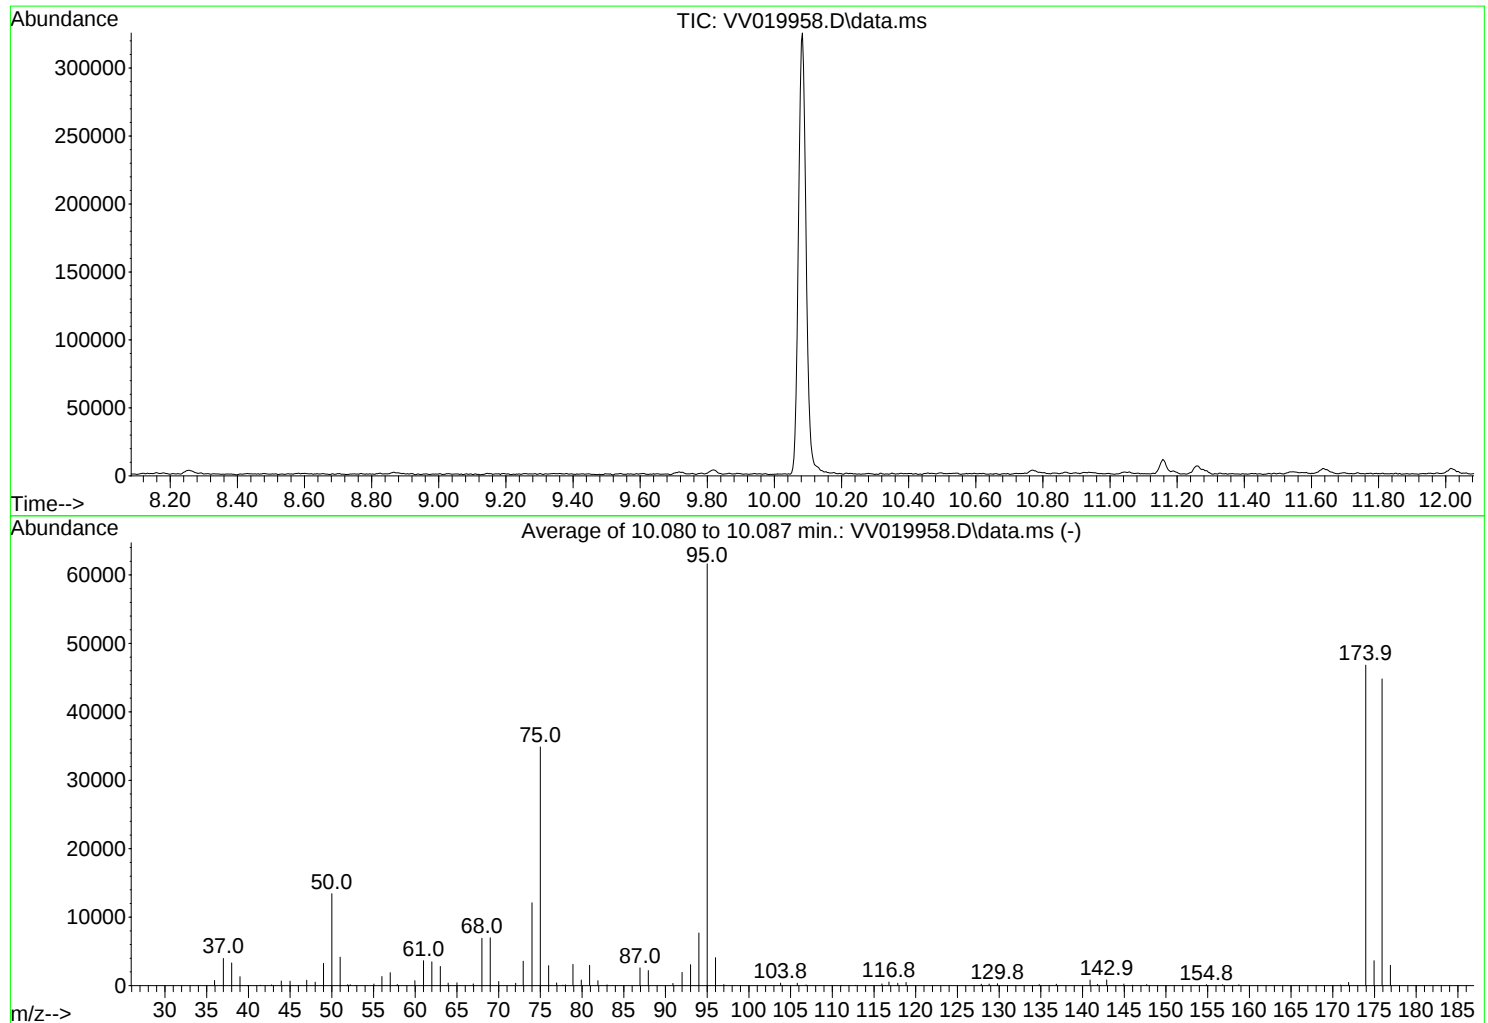

AutoFind: Scans 2796, 2797, 2798; Background Corrected with Scan 2785

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	13444	PASS
75	95	30	80	56.6	34891	PASS
95	95	100	100	100.0	61627	PASS
96	95	5	9	6.6	4095	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.0	46816	PASS
175	174	5	9	7.8	3646	PASS
176	174	95	101	95.7	44813	PASS
177	176	5	9	6.6	2967	PASS

m/z	Abundance
35.90	120.0
39.10	115.0
39.90	284.0
41.00	130.0
43.90	563.0
52.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	879.0
37.00	4103.0
38.00	3467.0
39.00	1604.0
39.90	335.0
42.80	101.0
44.00	1177.0
45.00	703.0
47.00	833.0
48.00	552.0
49.00	3240.0
50.00	13852.0
51.00	4371.0
51.90	214.0
52.90	102.0
55.00	199.0
56.00	1427.0
57.00	1923.0
57.80	151.0
59.90	800.0
61.00	3722.0
62.00	3583.0
63.00	2977.0
63.90	412.0
64.90	447.0
67.00	221.0
68.00	7097.0
69.00	7146.0
70.00	648.0
72.00	335.0
72.90	3597.0
74.00	12228.0
75.00	35648.0
76.00	3192.0
76.90	471.0
77.70	215.0
78.90	3211.0
79.90	774.0
80.90	2929.0
81.90	749.0
83.00	126.0
87.00	2428.0
88.00	2133.0
90.90	297.0
92.00	1844.0
93.00	3188.0
94.00	7790.0
95.00	62760.0
96.00	4294.0
97.00	198.0
103.80	353.0
105.80	361.0
106.80	114.0
111.10	102.0
116.00	245.0
116.80	543.0
117.80	354.0
118.90	496.0
127.80	205.0
128.80	240.0
129.70	255.0
134.80	170.0
136.80	163.0
140.90	829.0
141.80	189.0
142.90	842.0
144.90	201.0
146.00	102.0
147.70	169.0
154.90	159.0
156.80	144.0
158.80	141.0
171.00	150.0
171.90	461.0
174.00	46312.0
174.90	3680.0
175.90	44904.0
176.90	3065.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	893.0
37.00	4077.0
38.00	3425.0
39.00	1435.0
40.00	309.0
41.40	102.0
42.80	121.0
44.00	1274.0
45.00	681.0
47.00	842.0
48.00	544.0
49.00	3400.0
50.00	13808.0
51.00	4247.0
51.90	204.0
52.20	204.0
52.80	144.0
55.10	241.0
56.00	1386.0
57.00	1914.0
57.80	178.0
59.90	744.0
61.00	3722.0
62.00	3595.0
63.00	2867.0
63.90	386.0
65.00	423.0
66.90	280.0
68.00	7099.0
69.00	7260.0
70.00	632.0
72.00	331.0
73.00	3760.0
74.00	12492.0
75.00	36000.0
76.00	2978.0
76.90	395.0
78.00	163.0
78.90	3200.0
79.90	834.0
80.90	3027.0
81.90	756.0
83.10	117.0
87.00	2664.0
87.90	2232.0
90.90	340.0
92.00	1973.0
93.00	3075.0
94.00	7987.0
95.00	63968.0
96.00	4222.0
97.00	162.0
103.80	385.0
105.80	366.0
106.90	140.0
116.00	250.0
116.80	543.0
117.90	356.0
118.90	473.0
127.80	222.0
128.80	239.0
129.80	273.0
134.80	178.0
136.80	234.0
140.90	843.0
141.80	194.0
142.90	847.0
144.90	249.0
146.00	111.0
147.70	166.0
154.90	143.0
156.80	144.0
158.70	142.0
170.90	128.0
171.90	453.0
173.90	48528.0
174.90	3784.0
175.90	46216.0
176.90	3044.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	827.0
37.00	3754.0
38.00	3043.0
39.00	1222.0
40.00	241.0
41.40	107.0
42.80	125.0
44.00	1243.0
45.00	589.0
47.00	742.0
48.00	471.0
49.00	3092.0
50.00	12673.0
51.00	3886.0
52.20	205.0
52.80	132.0
55.00	246.0
56.00	1169.0
57.00	1850.0
57.90	168.0
60.00	644.0
61.00	3468.0
62.00	3268.0
63.00	2572.0
64.00	313.0
65.10	391.0
66.90	289.0
68.00	6581.0
69.00	6535.0
70.00	570.0
72.10	361.0
73.00	3364.0
74.00	11606.0
75.00	33024.0
76.00	2609.0
77.00	304.0
78.00	190.0
78.90	2948.0
79.90	853.0
80.90	2918.0
81.90	689.0
82.90	108.0
86.90	2695.0
87.90	2225.0
90.90	349.0
92.00	1972.0
93.00	2929.0
94.00	7286.0
95.00	58152.0
96.00	3770.0
97.00	134.0
103.80	372.0
105.80	354.0
106.90	118.0
112.80	132.0
115.90	271.0
116.80	512.0
117.90	358.0
118.80	423.0
127.90	228.0
128.80	227.0
129.90	328.0
134.80	154.0
136.90	255.0
140.90	779.0
141.80	164.0
142.90	853.0
145.00	234.0
147.70	173.0
154.80	167.0
156.80	126.0
158.70	117.0
171.90	467.0
173.90	45608.0
175.00	3475.0
175.90	43320.0
176.90	2792.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78