

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011124\
 Data File : VV033580.D
 Acq On : 11 Jan 2024 12:23
 Operator : SY/MD
 Sample : 05787-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jan 11 20:44:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 11 20:44:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	302003	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	283451	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	136163	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	105357	45.392	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.780%
7) Chloroethane-d5	1.532	69	92949	50.568	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	101.140%
11) 1,1-Dichloroethene-d2	2.063	65	49343	49.397	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.800%
21) 2-Butanone-d5	3.783	46	179091	112.493	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.490%
24) Chloroform-d	4.249	84	213645	51.477	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.960%
26) 1,2-Dichloroethane-d4	4.944	65	146667	54.694	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.380%
32) Benzene-d6	4.960	84	431364	53.530	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.060%
36) 1,2-Dichloropropane-d6	5.989	67	147319	55.539	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	111.080%
41) Toluene-d8	7.243	98	380396	52.392	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.780%
43) trans-1,3-Dichloroprop...	7.551	79	63755	48.633	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.260%
47) 2-Hexanone-d5	8.021	63	124436	113.096	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	113.100%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	183388	54.156	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	108.320%
66) 1,2-Dichlorobenzene-d4	11.561	152	144764	56.036	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.080%
Target Compounds						
44) trans-1,3-Dichloropropene	7.551	75	3312	0.939	ug/L	Qvalue # 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011124\
Data File : VV033580.D
Acq On : 11 Jan 2024 12:23
Operator : SY/MD
Sample : 05787-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jan 11 20:44:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 11 20:44:19 2024
Response via : Initial Calibration

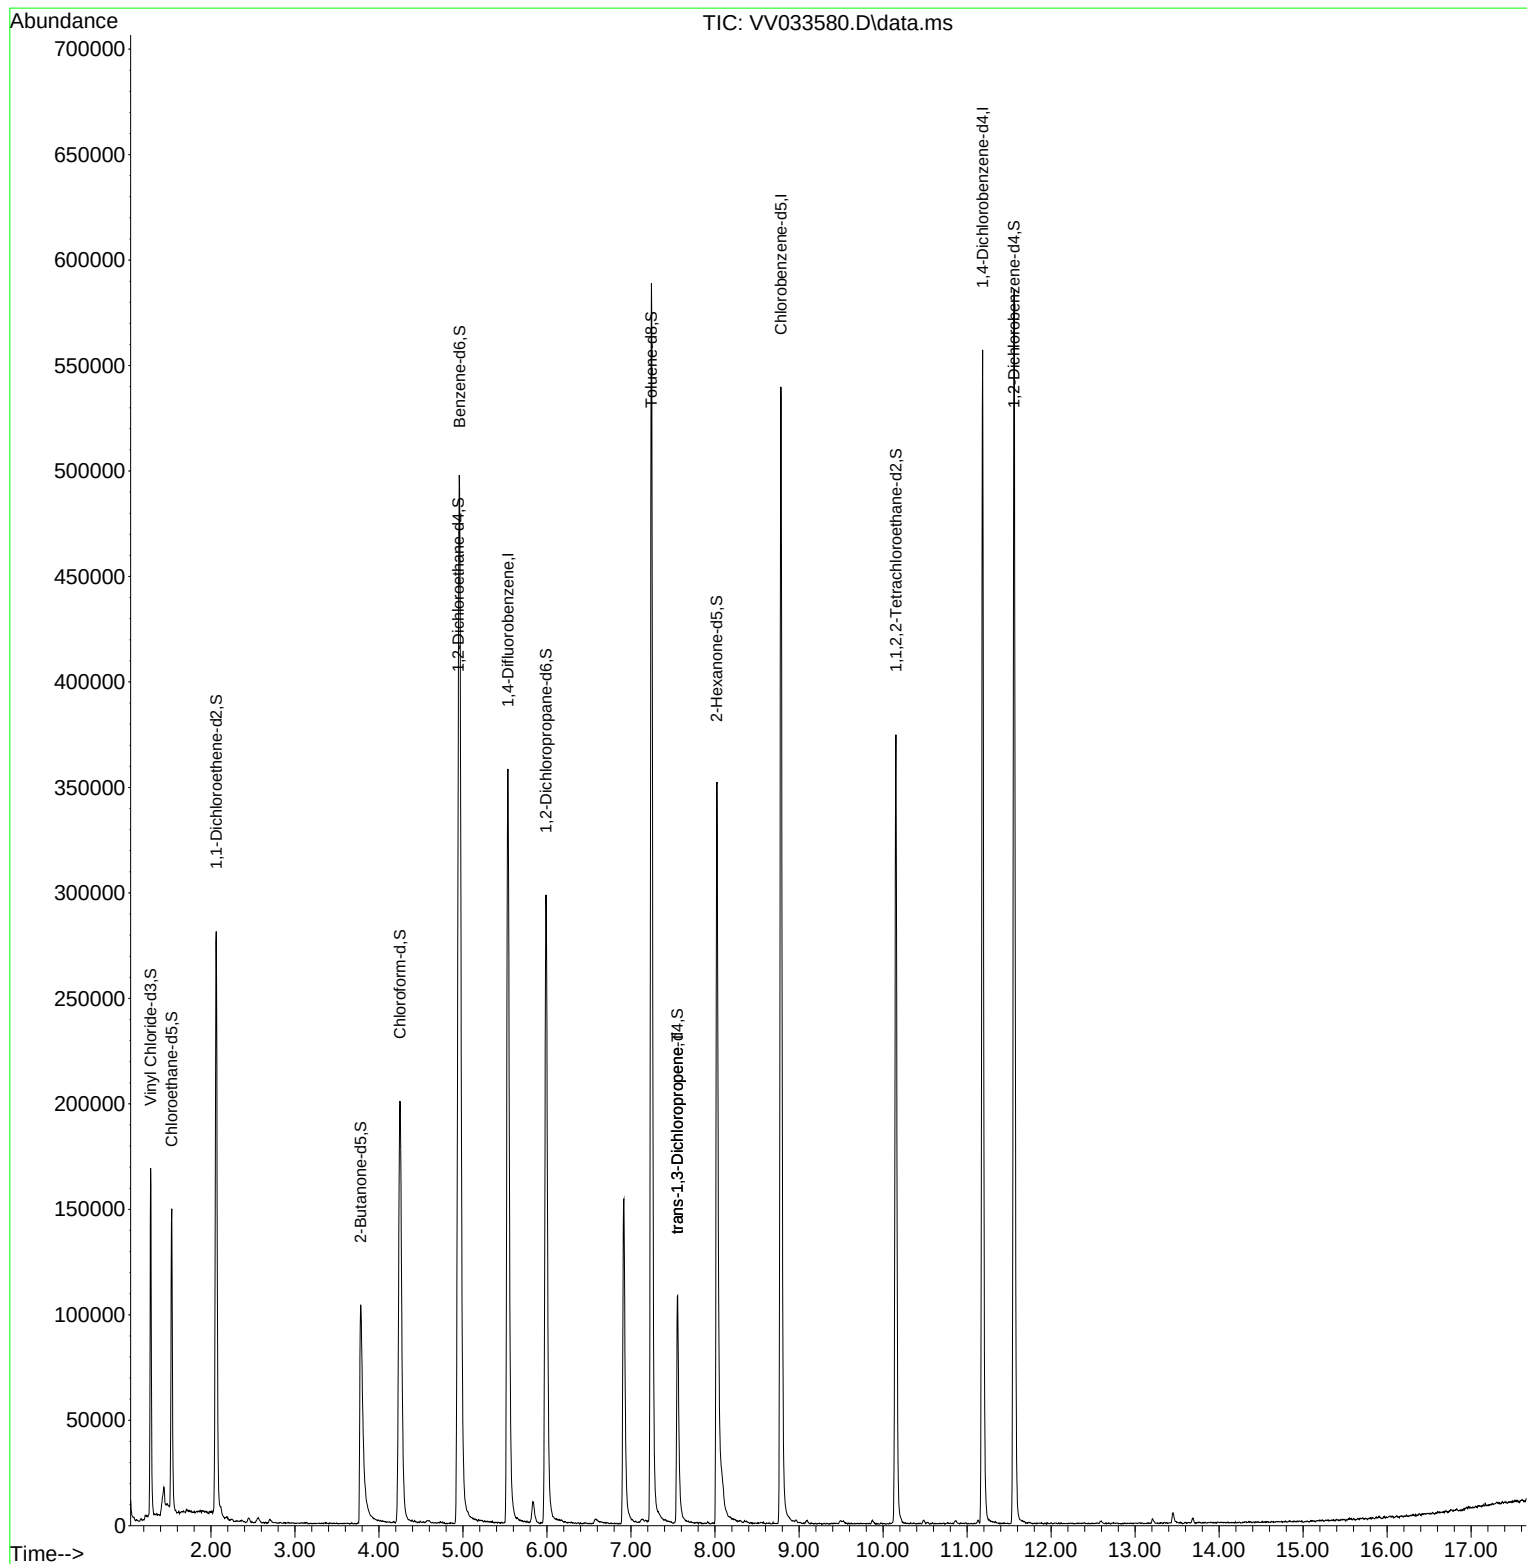

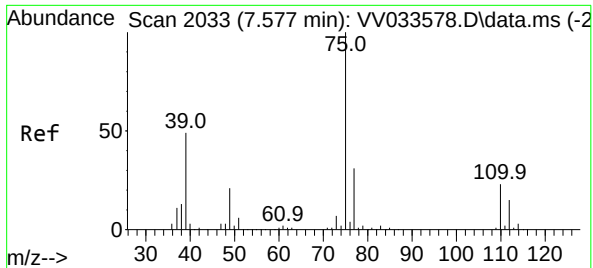

#44
 trans-1,3-Dichloropropene
 Concen: 0.939 ug/L
 RT: 7.551 min Scan# 20
 Delta R.T. -0.026 min
 Lab File: VV033580.D
 Acq: 11 Jan 2024 12:23

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 3312
 Ion Ratio Lower Upper
 75 100
 77 43.6 21.6 40.0#

