
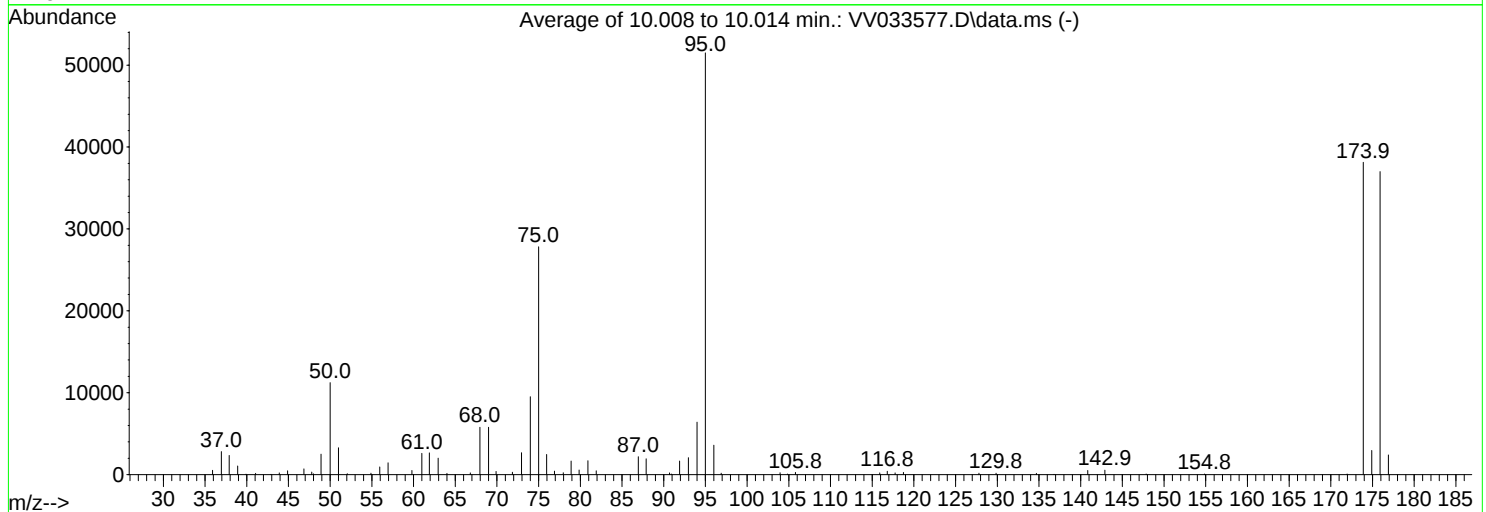


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011124\
Data File : VV033577.D
Acq On : 11 Jan 2024 10:27
Operator : SY/MD
Sample : BFB253
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB253

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM011024WMA.M
Title : VOC Analysis
Last Update : Thu Jan 11 20:44:19 2024

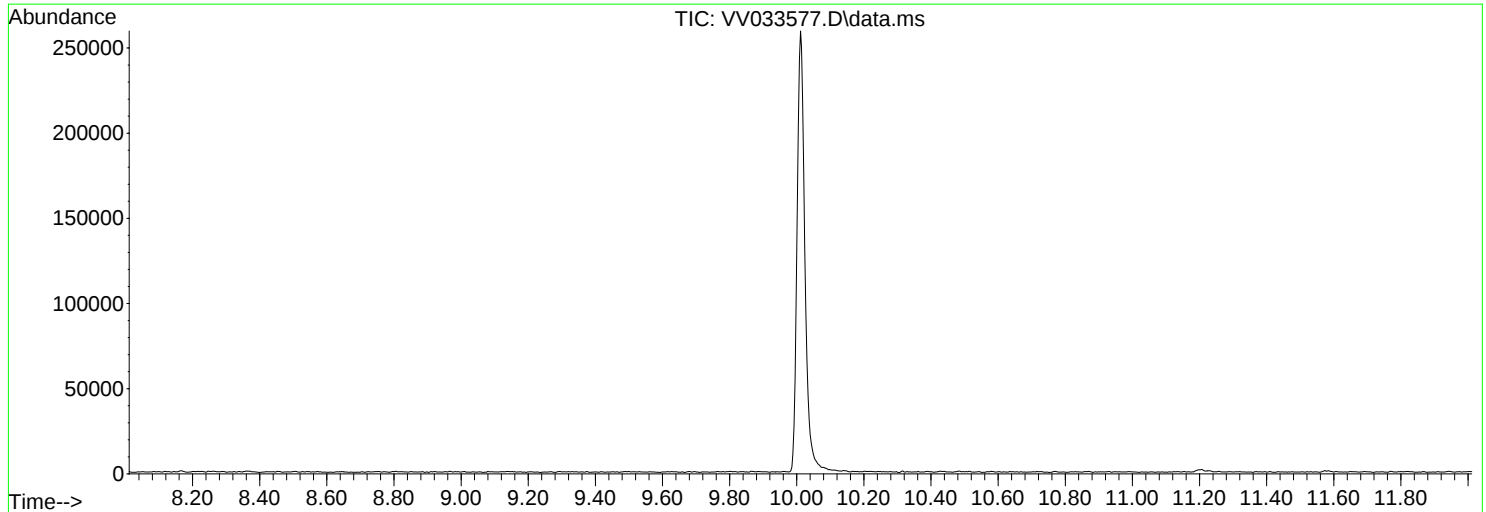

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	11241	PASS
75	95	30	80	54.0	27821	PASS
95	95	100	100	100.0	51499	PASS
96	95	5	9	7.0	3595	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.0	38125	PASS
175	174	5	9	7.7	2943	PASS
176	174	95	105	97.1	37005	PASS
177	176	5	10	6.5	2396	PASS

m/z	Abundance
39.90	188.0
40.90	253.0
43.00	154.0
43.90	388.0
55.00	112.0
57.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
35.90	609.0
36.90	2890.0
37.90	2275.0
38.90	1009.0
39.90	281.0
40.80	165.0
41.10	168.0
42.90	200.0
43.90	652.0
44.90	473.0
46.90	694.0
47.80	314.0
48.00	328.0
48.90	2479.0
50.00	11065.0
51.00	3232.0
52.00	130.0
54.90	269.0
56.00	892.0
56.90	1527.0
59.80	513.0
61.00	2491.0
61.90	2712.0
63.00	1869.0
63.90	179.0
66.80	205.0
67.90	5594.0
69.00	5807.0
69.90	384.0
71.80	275.0
73.00	2587.0
74.00	9240.0
75.00	27240.0
76.00	2568.0
76.90	426.0
78.00	223.0
78.90	1616.0
79.90	617.0
80.90	1752.0
81.90	455.0
86.90	2065.0
87.90	1957.0
90.70	200.0
91.90	1568.0
92.90	2057.0
94.00	6061.0
95.00	49584.0
96.00	3501.0
96.90	190.0
104.00	235.0
104.80	109.0
105.80	256.0
115.90	180.0
116.80	416.0
117.80	212.0
118.80	268.0
127.80	153.0
129.90	176.0
134.70	119.0
140.90	459.0
142.90	518.0
147.80	117.0
154.80	141.0
172.00	131.0
173.90	36200.0
174.90	2912.0
175.90	34888.0
176.90	2370.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
35.90	522.0
36.90	2872.0
37.90	2401.0
38.90	1082.0
39.90	244.0
41.10	152.0
42.90	202.0
43.90	596.0
44.90	482.0
46.90	729.0
47.80	315.0
48.90	2612.0
50.00	11668.0
51.00	3427.0
52.00	125.0
54.90	292.0
56.00	959.0
56.90	1599.0
59.80	531.0
61.00	2673.0
61.90	2752.0
63.00	2062.0
64.00	160.0
66.80	217.0
68.00	5957.0
69.00	5914.0
69.90	407.0
71.90	289.0
72.90	2746.0
74.00	9863.0
75.00	28800.0
76.00	2539.0
76.90	447.0
77.90	242.0
78.90	1708.0
79.90	582.0
80.90	1755.0
81.90	499.0
86.90	2300.0
87.90	1999.0
90.70	210.0
91.90	1739.0
93.00	2122.0
94.00	6747.0
95.00	53480.0
96.00	3704.0
96.90	190.0
103.90	252.0
104.90	105.0
105.80	286.0
115.90	221.0
116.80	418.0
117.80	214.0
118.80	295.0
127.80	187.0
129.90	185.0
134.70	177.0
140.80	521.0
142.90	557.0
147.90	103.0
154.90	116.0
171.90	118.0
173.90	39448.0
174.90	3030.0
175.90	38368.0
176.90	2447.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
35.90	444.0
37.00	2669.0
37.90	2334.0
38.90	1098.0
39.90	225.0
41.00	145.0
42.90	176.0
44.00	550.0
44.90	440.0
46.80	668.0
47.80	318.0
48.90	2392.0
50.00	10989.0
51.00	3197.0
52.10	120.0
54.90	280.0
55.90	941.0
57.00	1512.0
59.80	510.0
61.00	2607.0
61.90	2485.0
62.90	2097.0
64.10	156.0
66.80	208.0
68.00	5799.0
69.00	5607.0
69.90	407.0
71.90	294.0
72.90	2677.0
74.00	9444.0
75.00	27424.0
75.90	2264.0
76.90	431.0
77.90	238.0
78.90	1653.0
79.80	512.0
80.90	1597.0
81.90	477.0
87.00	2195.0
87.90	1853.0
90.70	213.0
90.90	212.0
91.90	1656.0
93.00	2032.0
94.00	6415.0
95.00	51432.0
96.00	3581.0
96.90	151.0
103.90	233.0
105.80	270.0
115.90	222.0
116.80	381.0
117.70	205.0
118.70	268.0
127.80	204.0
129.80	188.0
134.70	172.0
136.80	106.0
140.80	525.0
142.90	543.0
173.90	38728.0
174.90	2887.0
175.90	37760.0
176.90	2372.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253