

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
 Data File : VV033590.D
 Acq On : 12 Jan 2024 13:05
 Operator : SY/MD
 Sample : VV0112WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK391

Quant Time: Jan 12 23:42:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 12 23:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	141056	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	129151	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	62796	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	37410	4.850	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.000%
7) Chloroethane-d5	1.532	69	34241	5.005	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.200%
11) 1,1-Dichloroethene-d2	2.060	65	17595	5.062	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.200%
20) 2-Butanone-d5	3.834	46	91395	48.462	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.920%
24) Chloroform-d	4.252	84	80972	4.854	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%
26) 1,2-Dichloroethane-d4	4.947	65	39810	5.323	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.400%
32) Benzene-d6	4.963	84	160439	5.148	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
36) 1,2-Dichloropropane-d6	5.992	67	53260	5.126	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.600%
41) Toluene-d8	7.246	98	143510	5.158	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
43) trans-1,3-Dichloroprop...	7.561	79	18712	5.210	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.200%
46) 2-Hexanone-d5	8.030	63	71958	51.027	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.060%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	31169	5.134	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.600%
66) 1,2-Dichlorobenzene-d4	11.561	152	49603	5.145	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	2501	0.213	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033590.D
Acq On : 12 Jan 2024 13:05
Operator : SY/MD
Sample : VV0112WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK391

Quant Time: Jan 12 23:42:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 12 23:30:52 2024
Response via : Initial Calibration

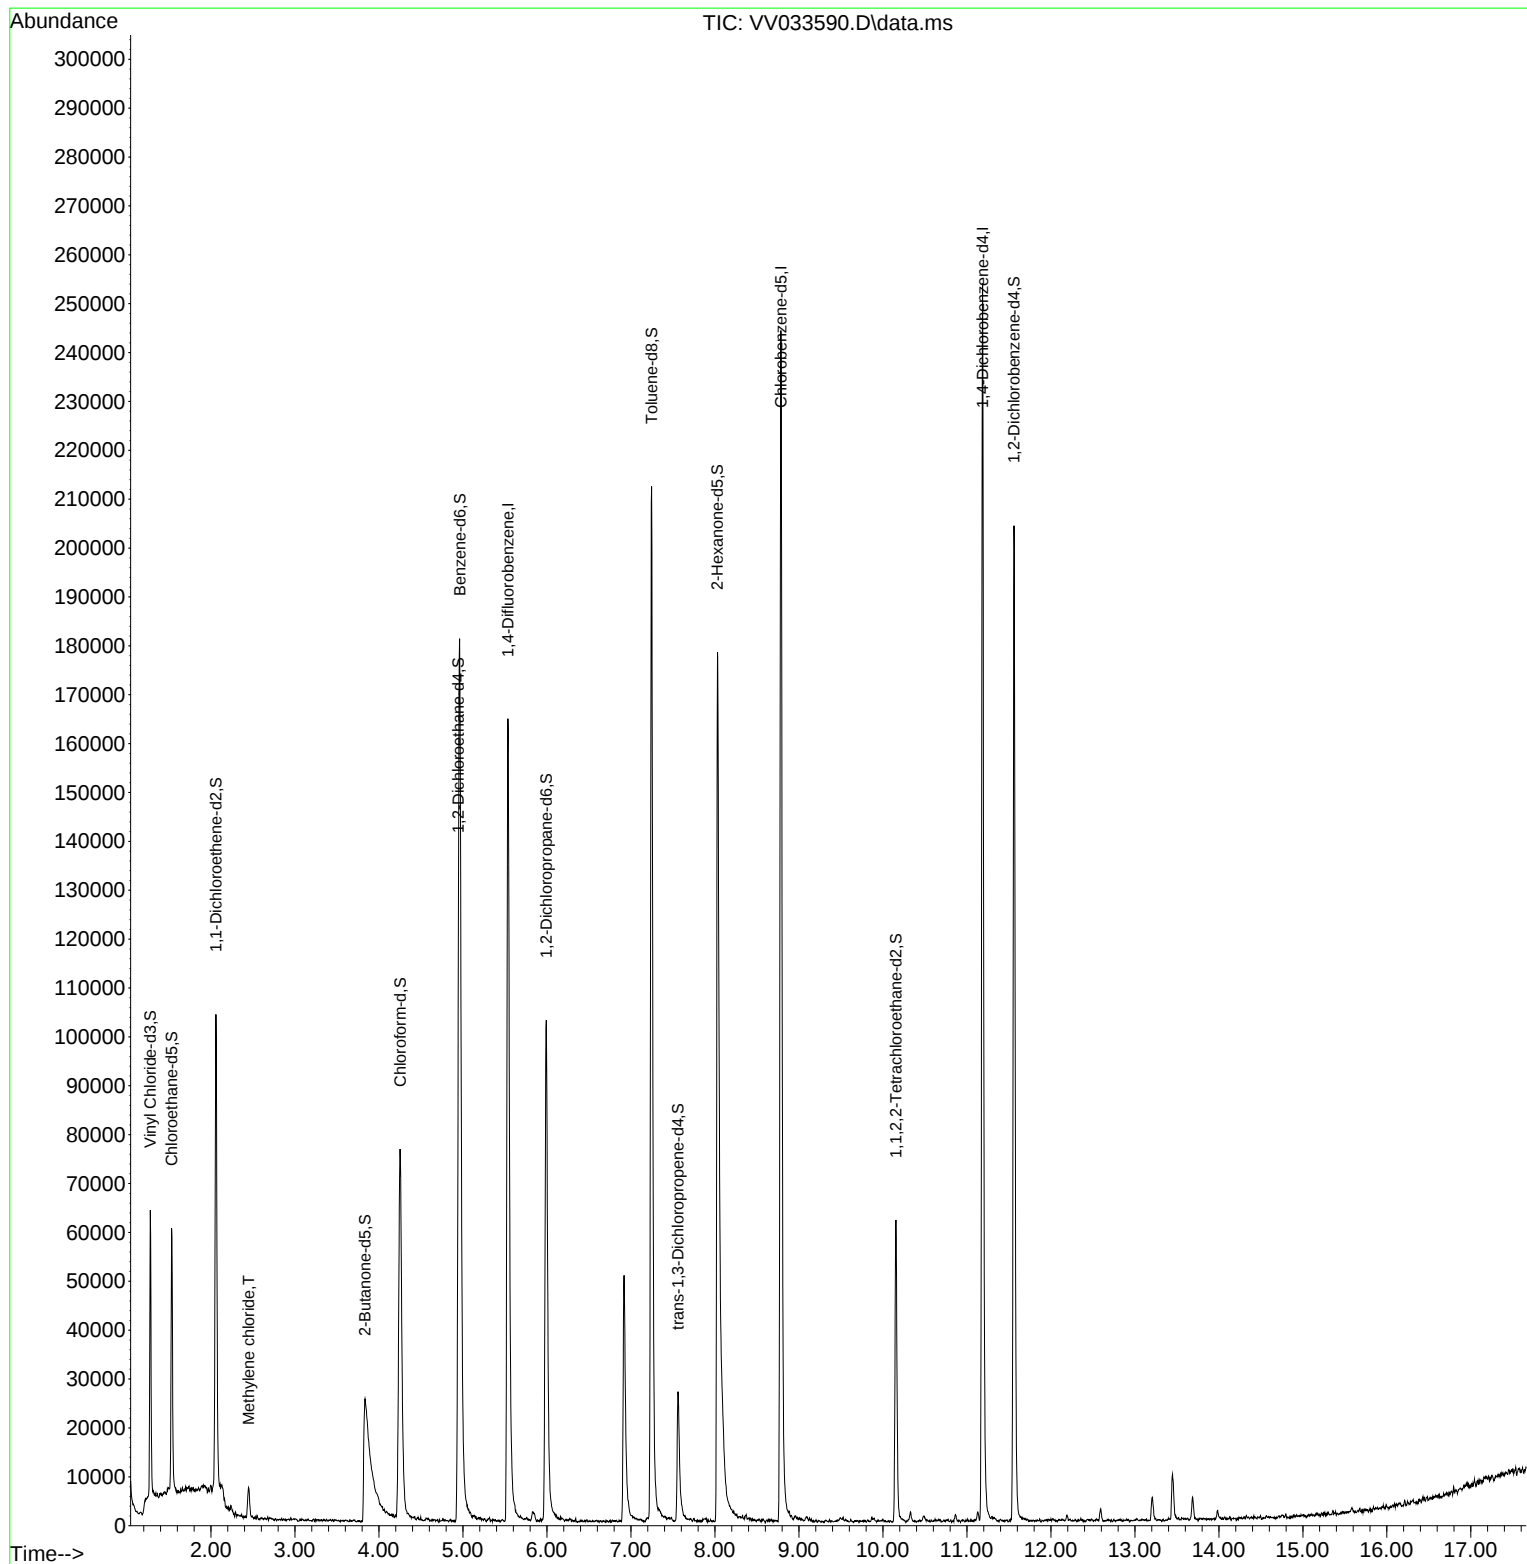

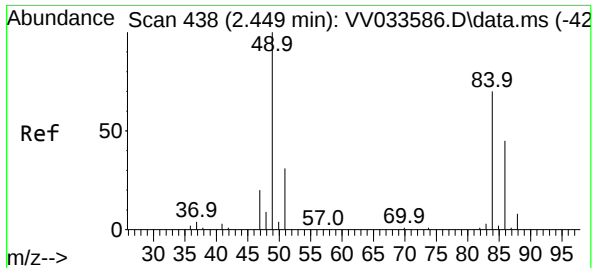

#16
Methylene chloride
Concen: 0.213 ug/L
RT: 2.449 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV033590.D
Acq: 12 Jan 2024 13:05

Instrument :
MSVOA_V
ClientSampleId :
VBLK391

Tgt Ion: 84 Resp: 2501

Ion	Ratio	Lower	Upper
84	100		
86	68.1	45.5	84.5
49	134.9	100.3	186.3

