

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
 Data File : VV033591.D
 Acq On : 12 Jan 2024 13:34
 Operator : SY/MD
 Sample : P1108-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ7

Quant Time: Jan 12 23:43:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 12 23:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	144177	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	128650	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	62386	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	36151	4.585	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.800%
7) Chloroethane-d5	1.532	69	33854	4.842	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.800%
11) 1,1-Dichloroethene-d2	2.060	65	16902	4.757	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.200%
20) 2-Butanone-d5	3.828	46	81390	42.223	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.440%
24) Chloroform-d	4.249	84	79977	4.691	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	4.944	65	37448	4.899	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.000%
32) Benzene-d6	4.960	84	158238	5.098	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
36) 1,2-Dichloropropane-d6	5.989	67	50269	4.857	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.200%
41) Toluene-d8	7.246	98	136566	4.928	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.600%
43) trans-1,3-Dichloroprop...	7.561	79	16313	4.559	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%
46) 2-Hexanone-d5	8.031	63	64427	45.864	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.720%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	28673	4.742	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	48312	5.044	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	3982	0.332	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033591.D
Acq On : 12 Jan 2024 13:34
Operator : SY/MD
Sample : P1108-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ7

Quant Time: Jan 12 23:43:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 12 23:30:52 2024
Response via : Initial Calibration

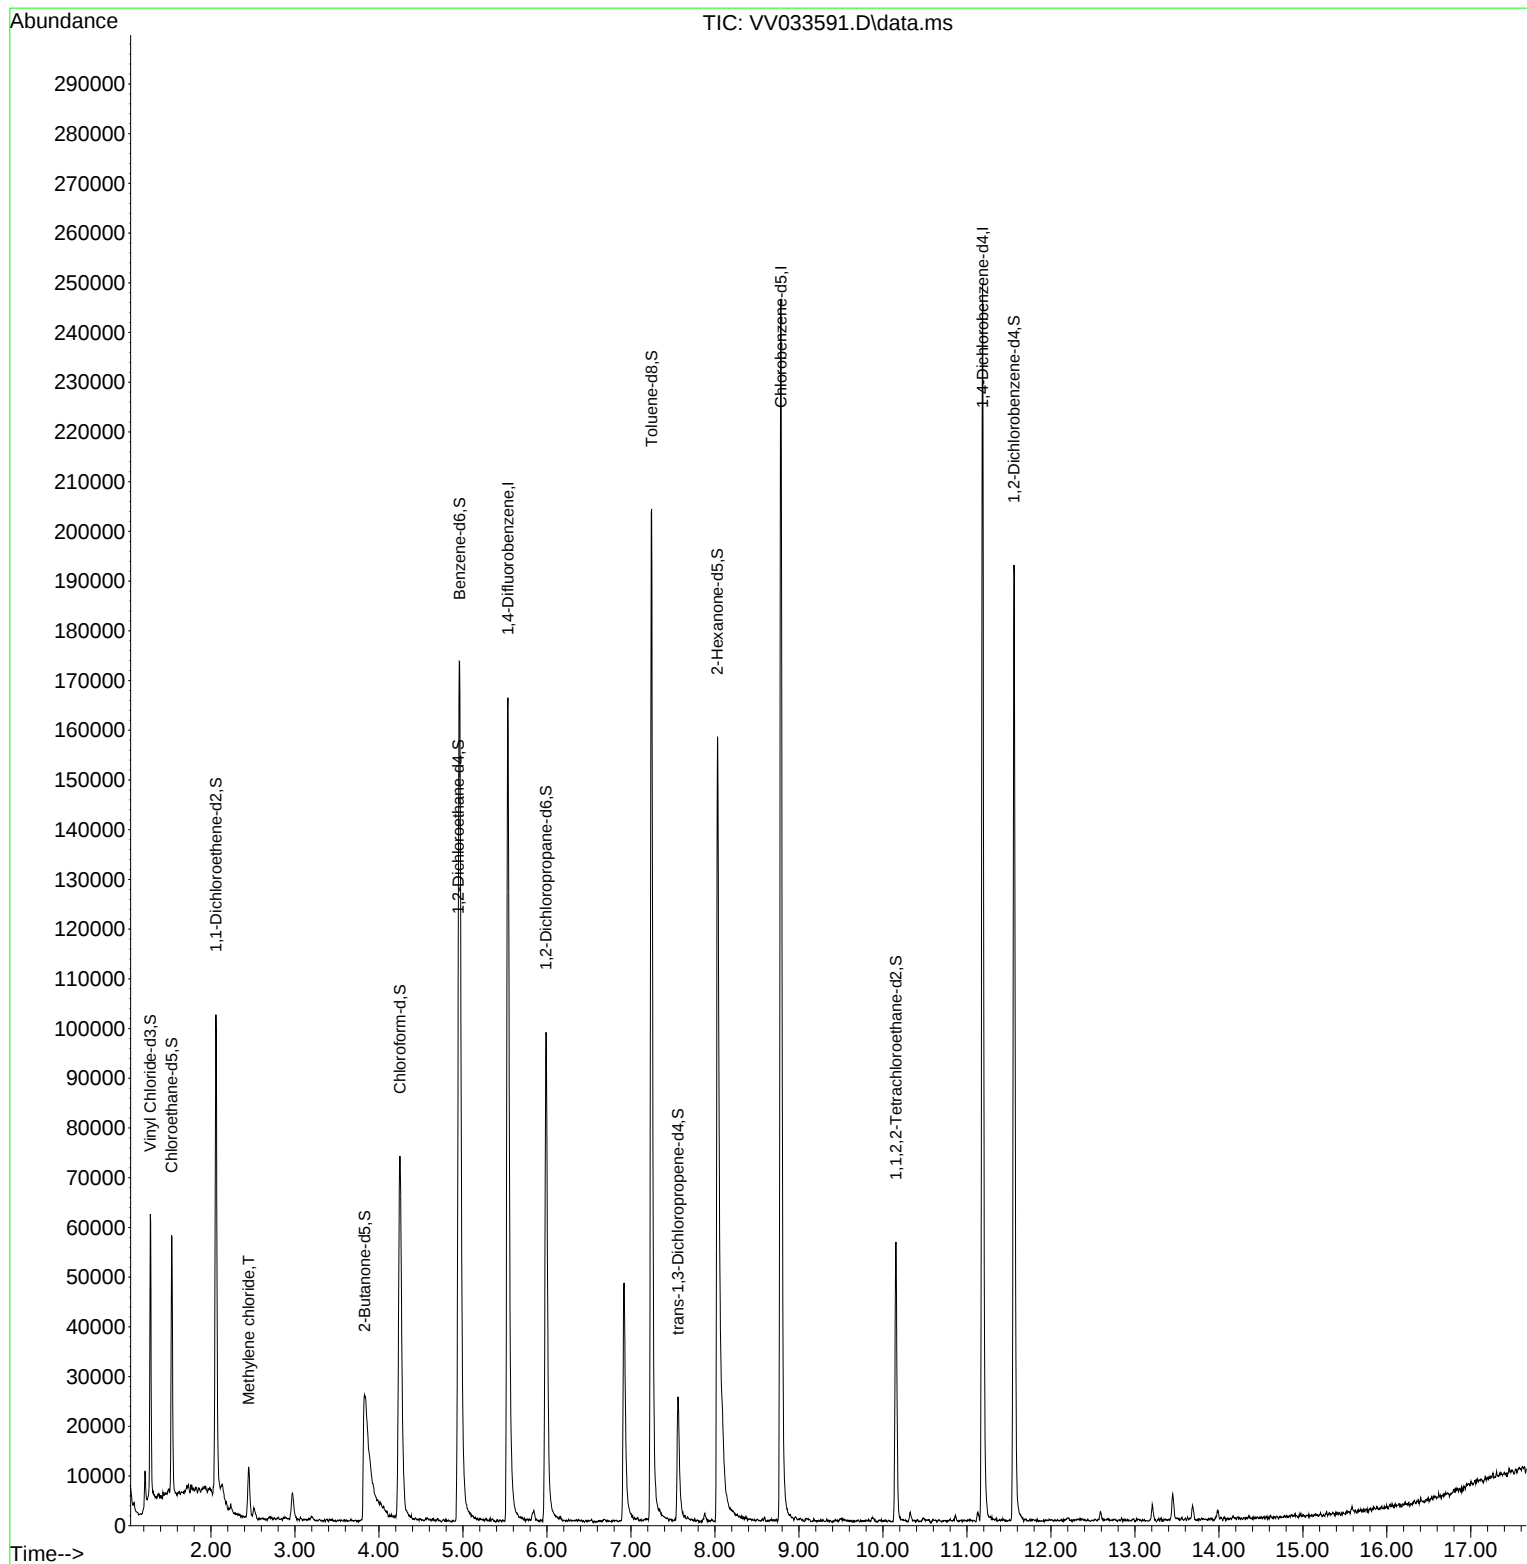

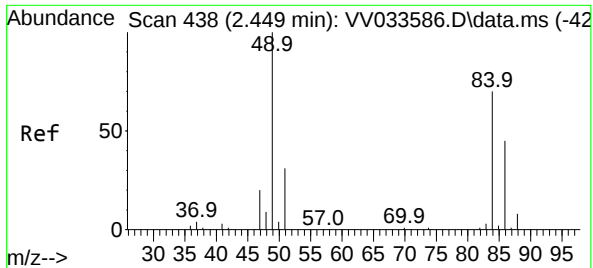

#16
Methylene chloride
Concen: 0.332 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV033591.D
Acq: 12 Jan 2024 13:34

Instrument :
MSVOA_V
ClientSampleId :
C0AZ7

Tgt Ion: 84 Resp: 3982

Ion	Ratio	Lower	Upper
84	100		
86	64.8	45.5	84.5
49	139.3	100.3	186.3

