

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011224\
 Data File : VW033599.D
 Acq On : 12 Jan 2024 16:44
 Operator : SY/MD
 Sample : P1108-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY9

Quant Time: Jan 12 23:46:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 12 23:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	130383	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	120726	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	61091	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	33885	4.753	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.000%
7) Chloroethane-d5	1.536	69	30252	4.784	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.600%
11) 1,1-Dichloroethene-d2	2.063	65	15770	4.908	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.200%
20) 2-Butanone-d5	3.802	46	86199	49.449	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.900%
24) Chloroform-d	4.253	84	74517	4.833	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.600%
26) 1,2-Dichloroethane-d4	4.947	65	35182	5.089	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.800%
32) Benzene-d6	4.963	84	144377	4.956	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	5.992	67	47032	4.843	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.800%
41) Toluene-d8	7.246	98	127920	4.919	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
43) trans-1,3-Dichloroprop...	7.561	79	16956	5.050	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.000%
46) 2-Hexanone-d5	8.027	63	66811	50.683	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.360%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	29923	5.273	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	46850	4.995	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds						
					Qvalue	
22) cis-1,2-Dichloroethene	3.818	96	1251	0.115	ug/L	87
51) Chlorobenzene	8.818	112	10469	0.377	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033599.D
Acq On : 12 Jan 2024 16:44
Operator : SY/MD
Sample : P1108-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY9

Quant Time: Jan 12 23:46:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 12 23:30:52 2024
Response via : Initial Calibration




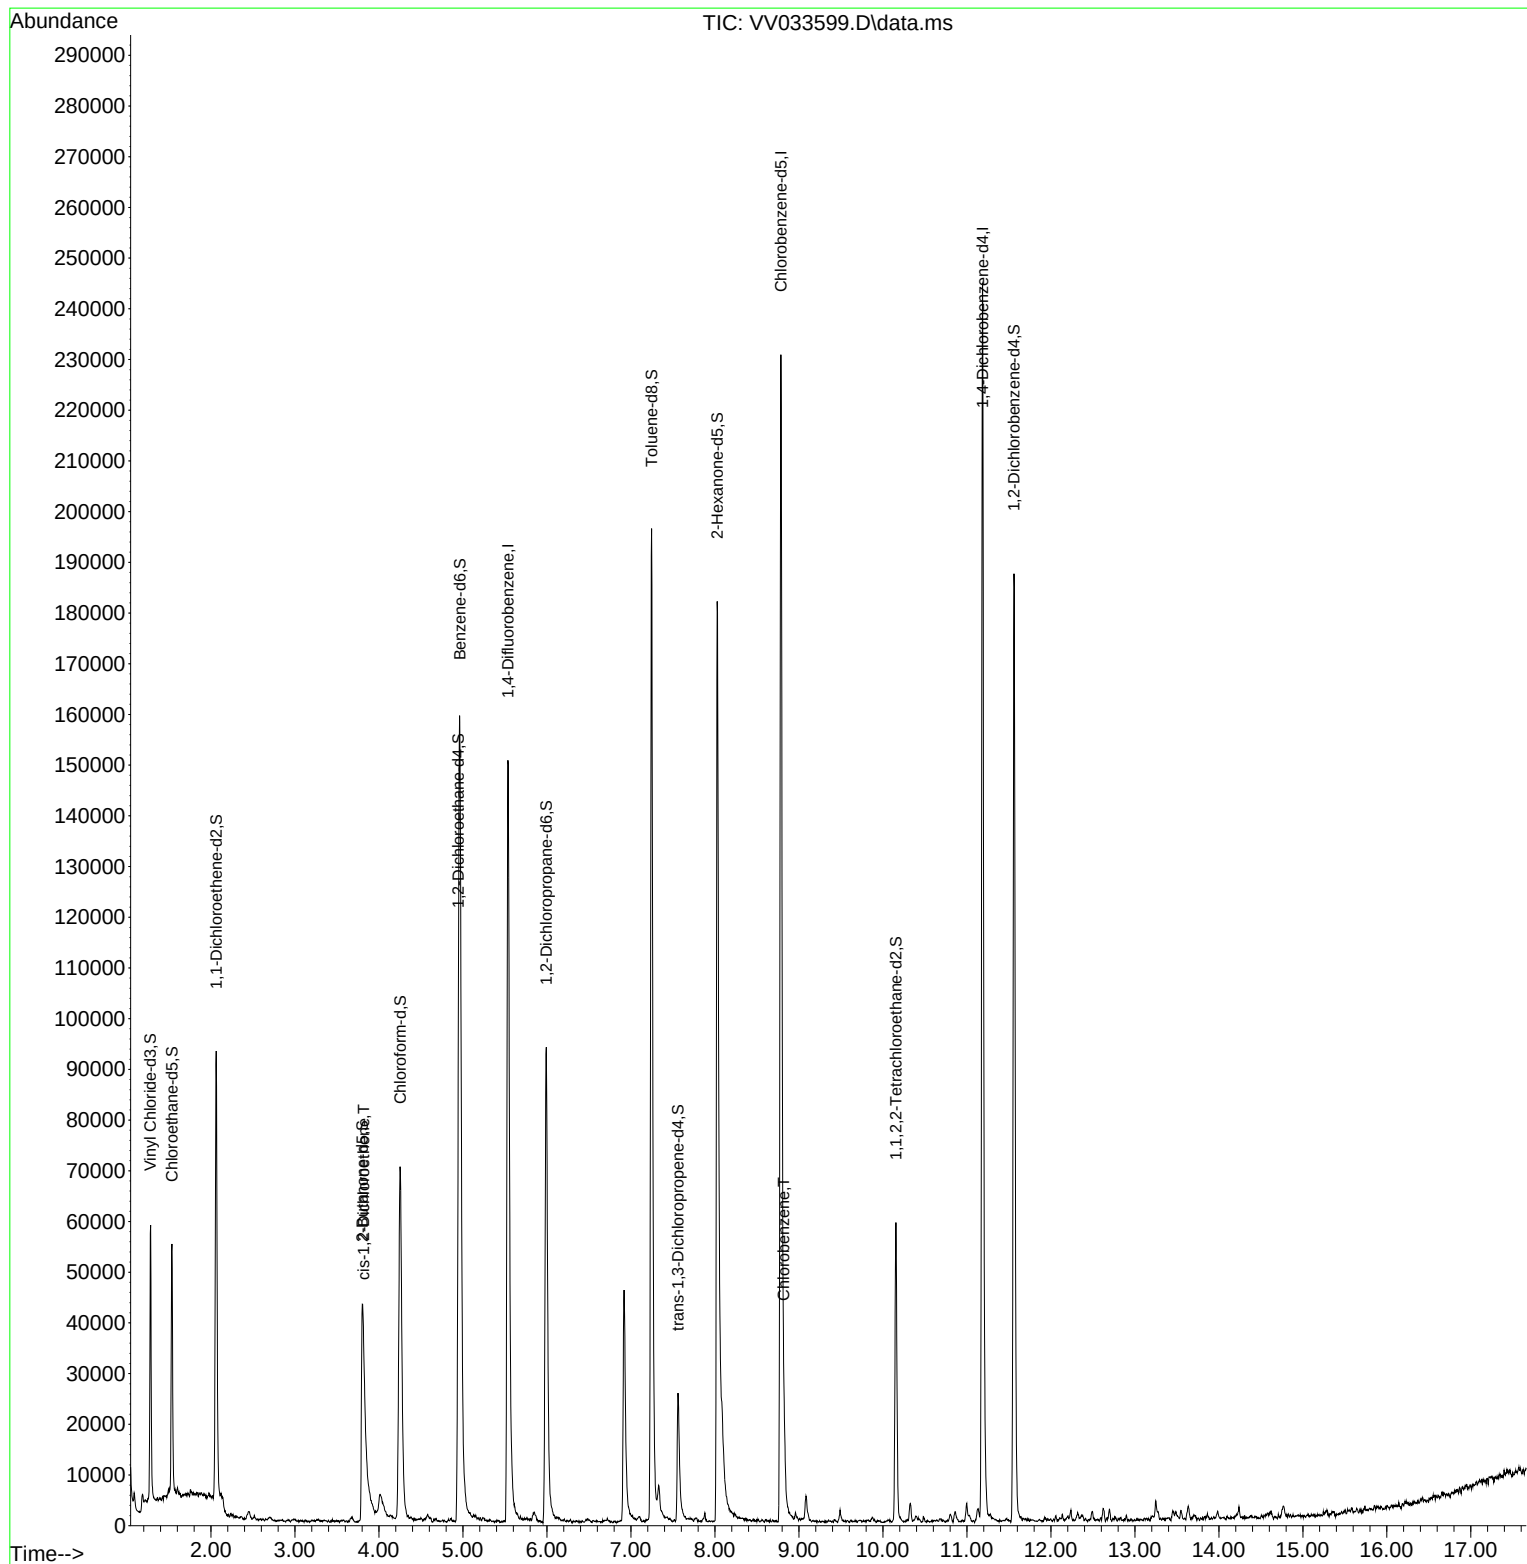


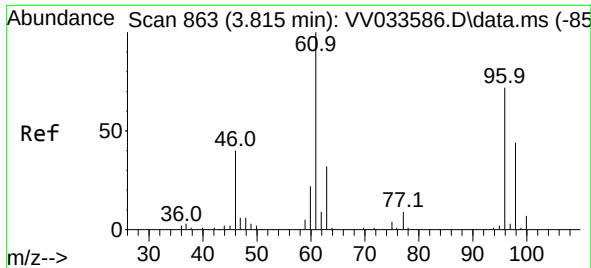

#22
 cis-1,2-Dichloroethene
 Concen: 0.115 ug/L
 RT: 3.818 min Scan# 863
 Delta R.T. 0.003 min
 Lab File: VV033599.D
 Acq: 12 Jan 2024 16:44

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY9

Tgt Ion:	96	Resp:	1251
Ion	Ratio	Lower	Upper
96	100		
61	119.9	97.1	180.3
98	55.2	42.6	79.0

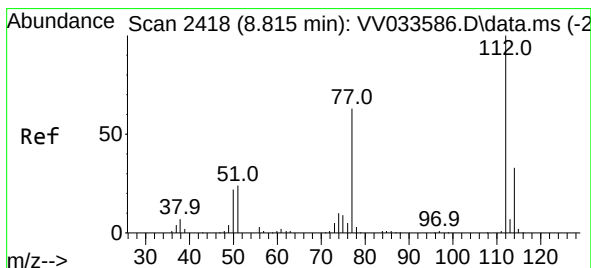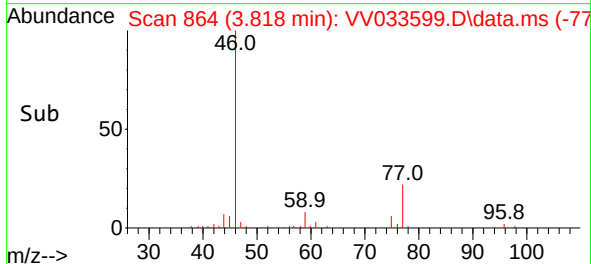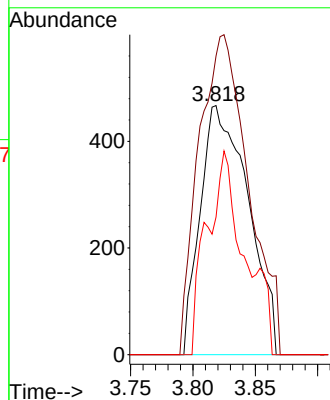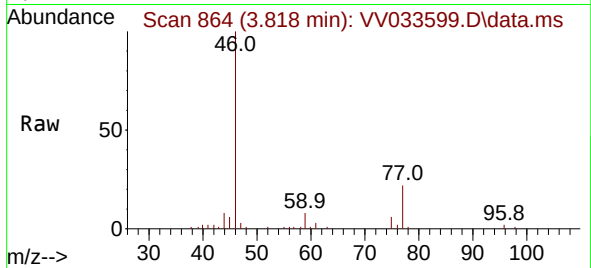

#51
 Chlorobenzene
 Concen: 0.377 ug/L
 RT: 8.818 min Scan# 2419
 Delta R.T. 0.003 min
 Lab File: VV033599.D
 Acq: 12 Jan 2024 16:44

Tgt Ion:	112	Resp:	10469
Ion	Ratio	Lower	Upper
112	100		
114	32.4	22.9	42.5
77	68.9	50.8	76.2

