

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
 Data File : VV033600.D
 Acq On : 12 Jan 2024 17:08
 Operator : SY/MD
 Sample : P1108-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ1

Quant Time: Jan 12 23:46:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 12 23:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	125308	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	115399	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	59242	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	31863	4.650	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.000%
7) Chloroethane-d5	1.532	69	29883	4.917	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.400%
11) 1,1-Dichloroethene-d2	2.060	65	14903	4.826	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.600%
20) 2-Butanone-d5	3.838	46	65300	38.977	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.960%
24) Chloroform-d	4.253	84	71850	4.849	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%
26) 1,2-Dichloroethane-d4	4.947	65	34545	5.199	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	4.963	84	138073	4.959	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	5.992	67	45252	4.875	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.400%
41) Toluene-d8	7.246	98	121974	4.907	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
43) trans-1,3-Dichloroprop...	7.561	79	16212	5.051	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.000%
46) 2-Hexanone-d5	8.031	63	63147	50.115	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.220%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	29320	5.405	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.200%
66) 1,2-Dichlorobenzene-d4	11.561	152	46126	5.071	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.400%
Target Compounds						
					Qvalue	
51) Chlorobenzene	8.818	112	19170	0.722	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033600.D
Acq On : 12 Jan 2024 17:08
Operator : SY/MD
Sample : P1108-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ1

Quant Time: Jan 12 23:46:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 12 23:30:52 2024
Response via : Initial Calibration

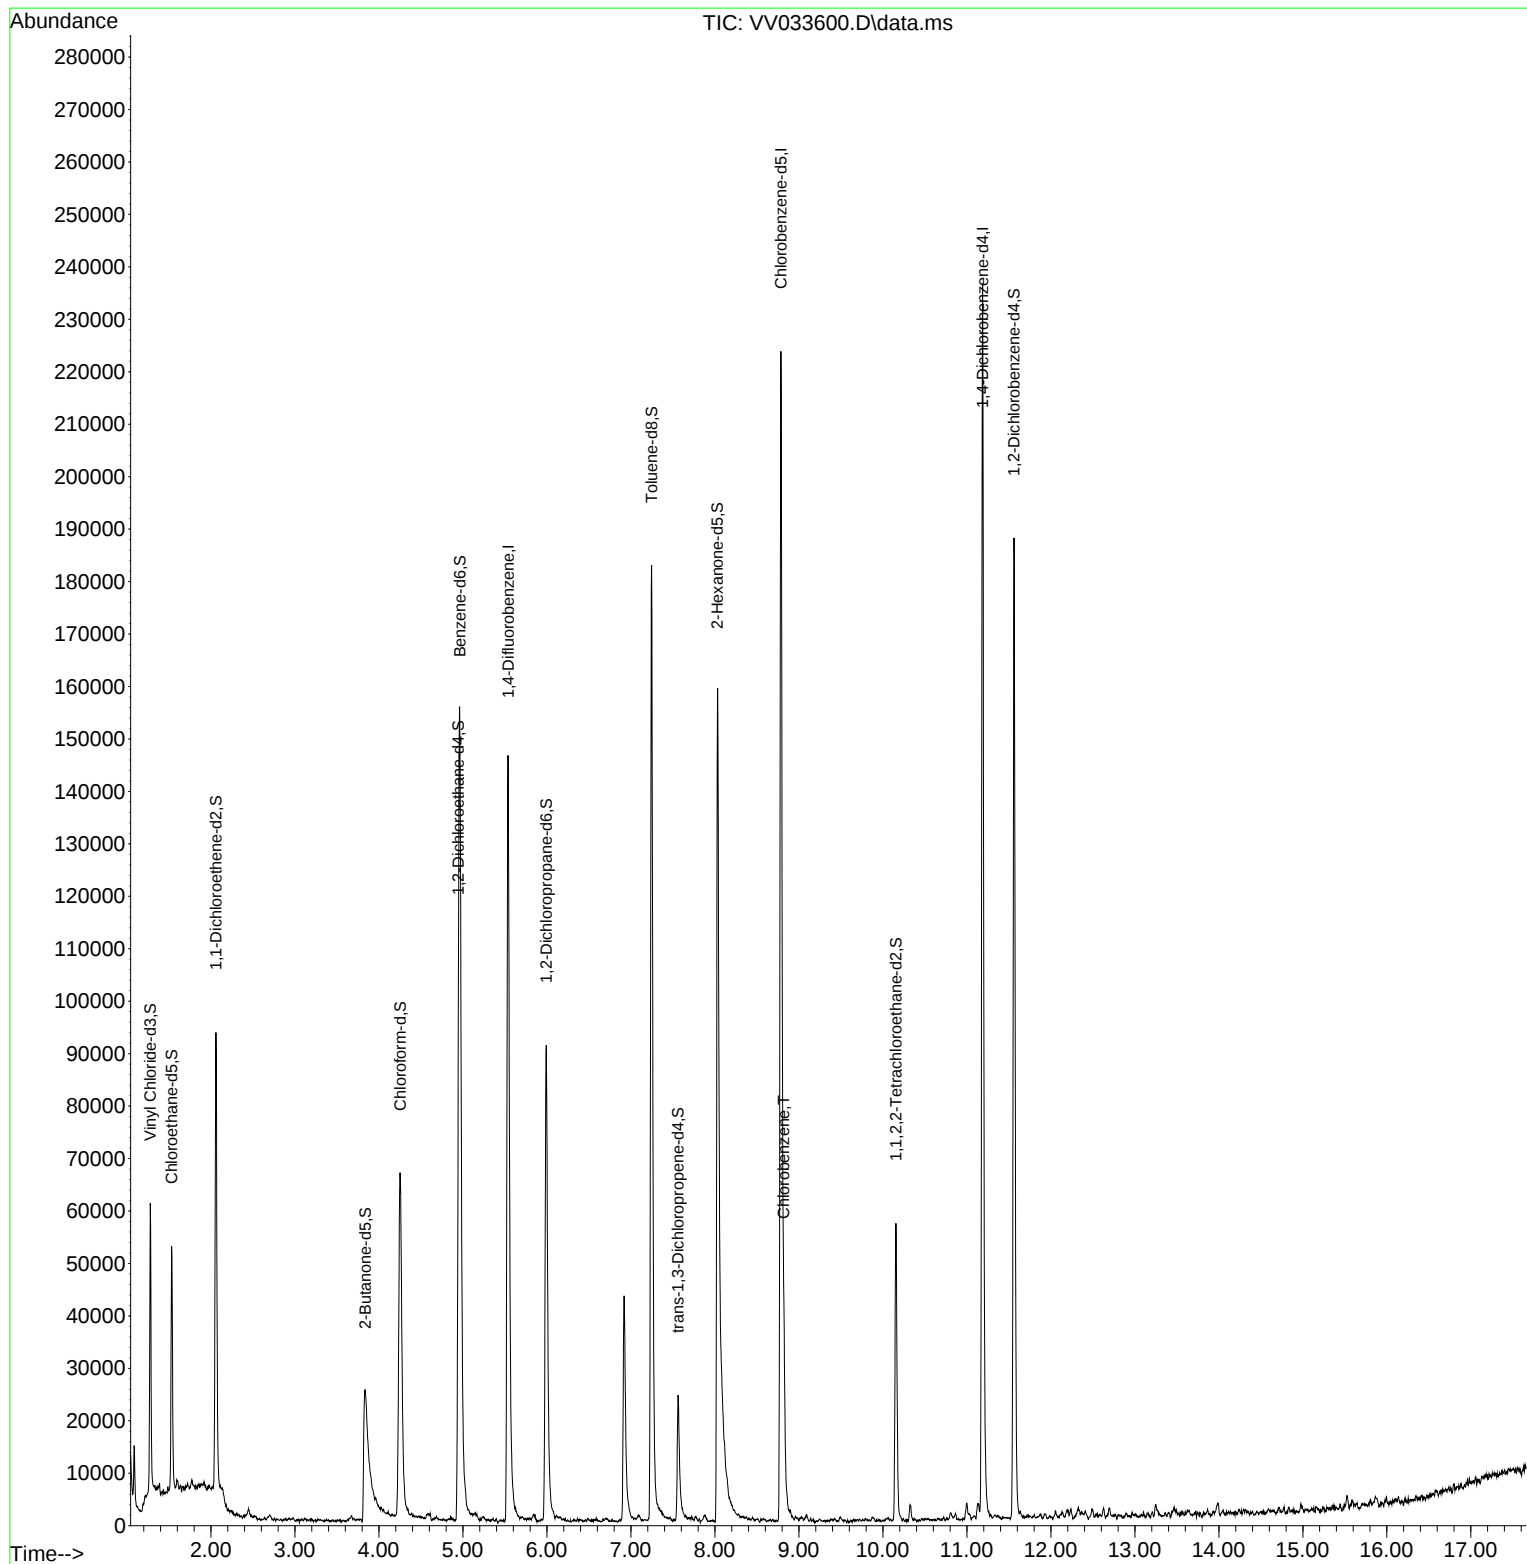

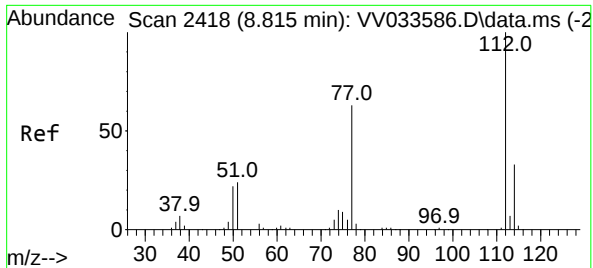

#51
 Chlorobenzene
 Concen: 0.722 ug/L
 RT: 8.818 min Scan# 2419
 Delta R.T. 0.003 min
 Lab File: VV033600.D
 Acq: 12 Jan 2024 17:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ1

Tgt Ion:	112	Resp:	19170
Ion	Ratio	Lower	Upper
112	100		
114	31.9	22.9	42.5
77	63.5	50.8	76.2

