

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
 Data File : VV033604.D
 Acq On : 12 Jan 2024 18:43
 Operator : SY/MD
 Sample : P1108-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B38

Quant Time: Jan 12 23:48:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 12 23:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	127142	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	118987	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	59635	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	31610	4.546	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.000%
7) Chloroethane-d5	1.535	69	28720	4.658	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.200%
11) 1,1-Dichloroethene-d2	2.059	65	14670	4.682	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.600%
20) 2-Butanone-d5	3.815	46	86790	51.057	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.120%
24) Chloroform-d	4.252	84	70667	4.700	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
26) 1,2-Dichloroethane-d4	4.947	65	34775	5.159	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	4.963	84	139323	4.853	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%
36) 1,2-Dichloropropane-d6	5.992	67	45249	4.727	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%
41) Toluene-d8	7.246	98	121848	4.754	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.000%
43) trans-1,3-Dichloroprop...	7.561	79	15596	4.713	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.200%
46) 2-Hexanone-d5	8.027	63	64114	49.348	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.700%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	29006	5.186	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	45532	4.973	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.400%
Target Compounds					Qvalue	
13) Acetone	2.143	43	13072	9.473	ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033604.D
Acq On : 12 Jan 2024 18:43
Operator : SY/MD
Sample : P1108-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B38

Quant Time: Jan 12 23:48:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 12 23:30:52 2024
Response via : Initial Calibration

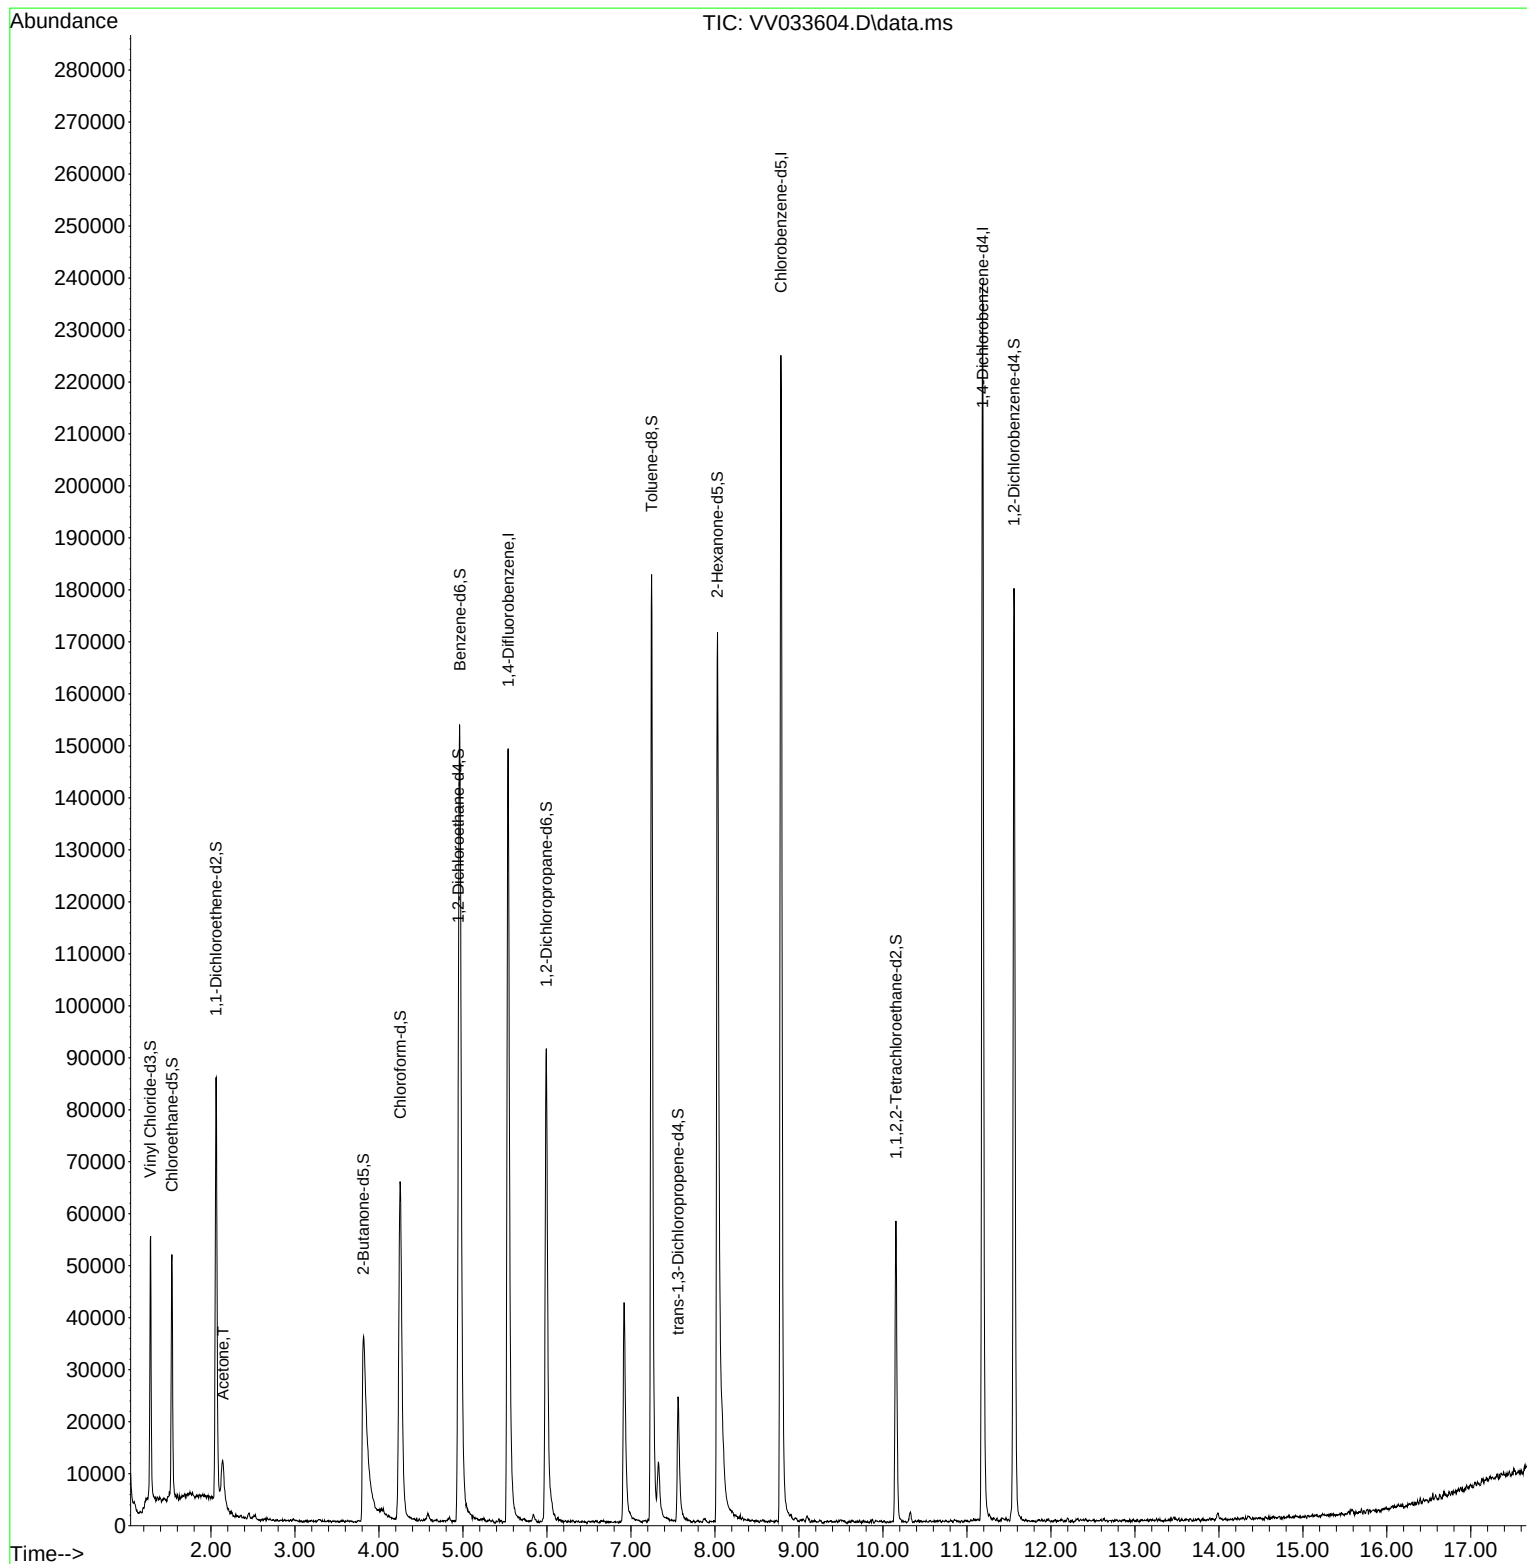

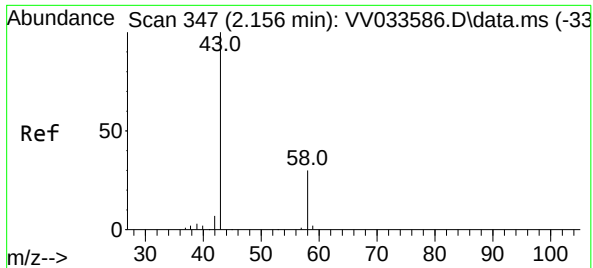

#13
 Acetone
 Concen: 9.473 ug/L
 RT: 2.143 min Scan# 34
 Delta R.T. -0.013 min
 Lab File: VV033604.D
 Acq: 12 Jan 2024 18:43

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B38

Tgt Ion: 43 Resp: 13072
 Ion Ratio Lower Upper
 43 100
 58 37.6 0.0 51.0

