

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011224\
 Data File : VW033605.D
 Acq On : 12 Jan 2024 19:07
 Operator : SY/MD
 Sample : P1108-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B45

Quant Time: Jan 12 23:48:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 12 23:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	125693	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	118091	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	59893	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	32400	4.714	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.200%
7) Chloroethane-d5	1.536	69	30113	4.940	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.800%
11) 1,1-Dichloroethene-d2	2.060	65	15626	5.045	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.800%
20) 2-Butanone-d5	3.818	46	90550	53.883	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.760%
24) Chloroform-d	4.253	84	74140	4.988	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	4.947	65	36858	5.531	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.600%
32) Benzene-d6	4.963	84	144015	5.054	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.000%
36) 1,2-Dichloropropane-d6	5.992	67	47478	4.998	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.000%
41) Toluene-d8	7.246	98	127387	5.008	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.200%
43) trans-1,3-Dichloroprop...	7.561	79	16968	5.166	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.400%
46) 2-Hexanone-d5	8.031	63	67768	52.556	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.120%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	30192	5.439	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	48319	5.254	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.000%
Target Compounds						Qvalue
34) Trichloroethene	5.847	95	2427	0.217	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033605.D
Acq On : 12 Jan 2024 19:07
Operator : SY/MD
Sample : P1108-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B45


Quant Time: Jan 12 23:48:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 12 23:30:52 2024
Response via : Initial Calibration

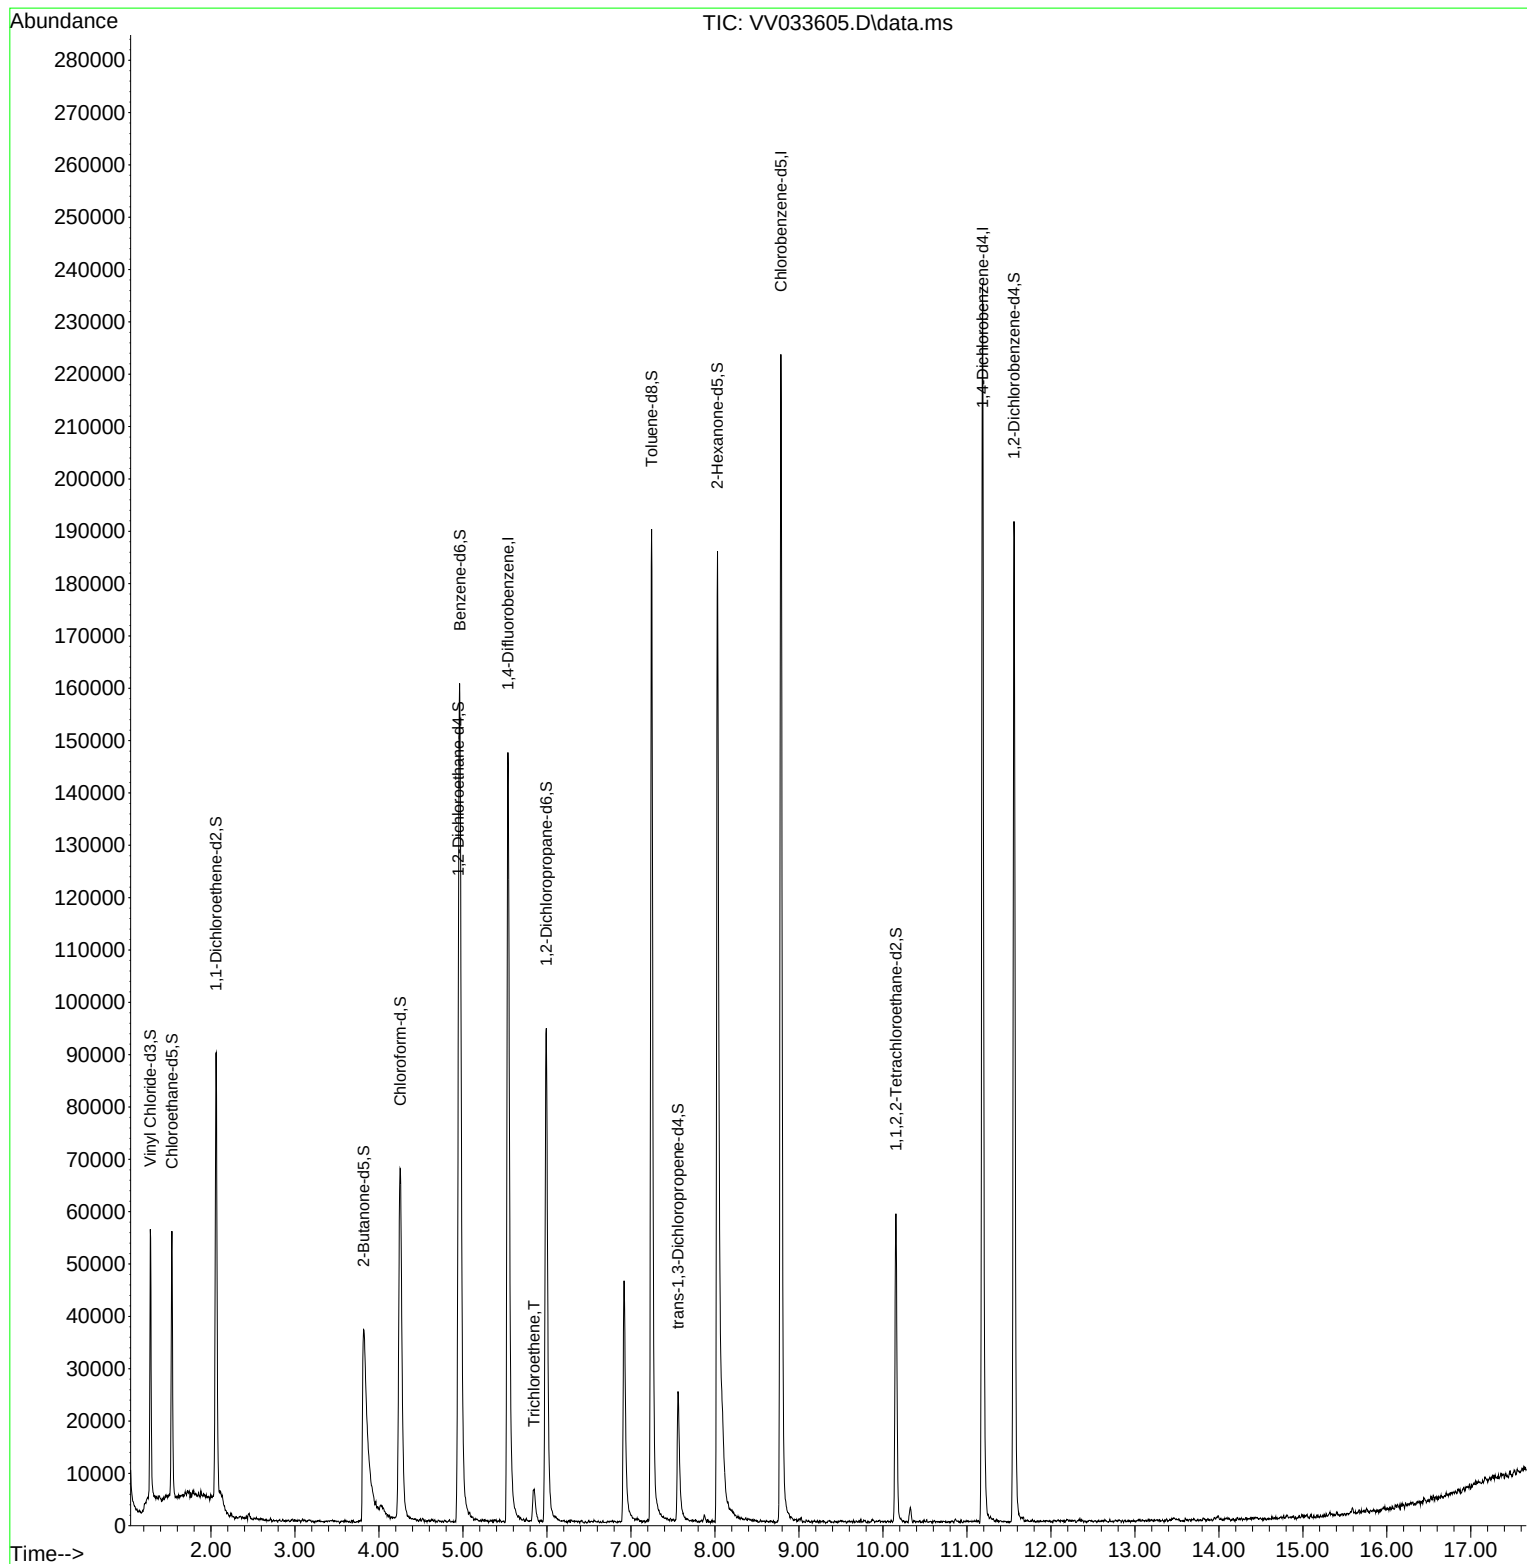

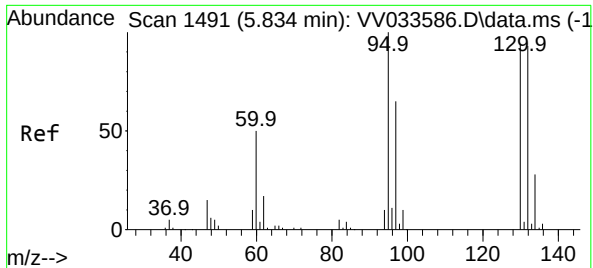

#34
 Trichloroethene
 Concen: 0.217 ug/L
 RT: 5.847 min Scan# 1495
 Delta R.T. 0.013 min
 Lab File: VV033605.D
 Acq: 12 Jan 2024 19:07

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B45

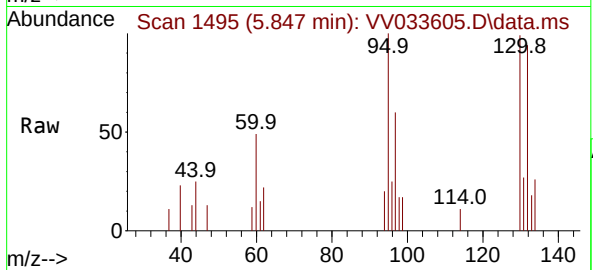

Tgt Ion:	95	Resp:	2427
Ion	Ratio	Lower	Upper
95	100		
97	60.4	45.1	83.9
132	94.2	65.2	121.2
130	99.5	66.0	122.6

