

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
 Data File : VV033608.D
 Acq On : 12 Jan 2024 20:42
 Operator : SY/MD
 Sample : VV0112WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK392

Quant Time: Jan 13 00:31:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jan 13 00:29:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	127434	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	118060	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	57477	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	33673	4.832	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.600%
7) Chloroethane-d5	1.536	69	31167	5.043	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.800%
11) 1,1-Dichloroethene-d2	2.063	65	15391	4.901	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.000%
20) 2-Butanone-d5	3.841	46	86845	50.972	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.940%
24) Chloroform-d	4.252	84	74664	4.955	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	4.950	65	37898	5.609	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.200%
32) Benzene-d6	4.963	84	147140	5.165	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
36) 1,2-Dichloropropane-d6	5.992	67	47839	5.037	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.246	98	126841	4.988	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
43) trans-1,3-Dichloroprop...	7.561	79	16619	5.061	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.200%
46) 2-Hexanone-d5	8.034	63	69173	53.660	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.320%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	30169	5.436	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	46100	5.224	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.400%
Target Compounds						Qvalue
16) Methylene chloride	2.452	84	2786	0.263	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033608.D
Acq On : 12 Jan 2024 20:42
Operator : SY/MD
Sample : VV0112WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK392

Quant Time: Jan 13 00:31:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jan 13 00:29:44 2024
Response via : Initial Calibration

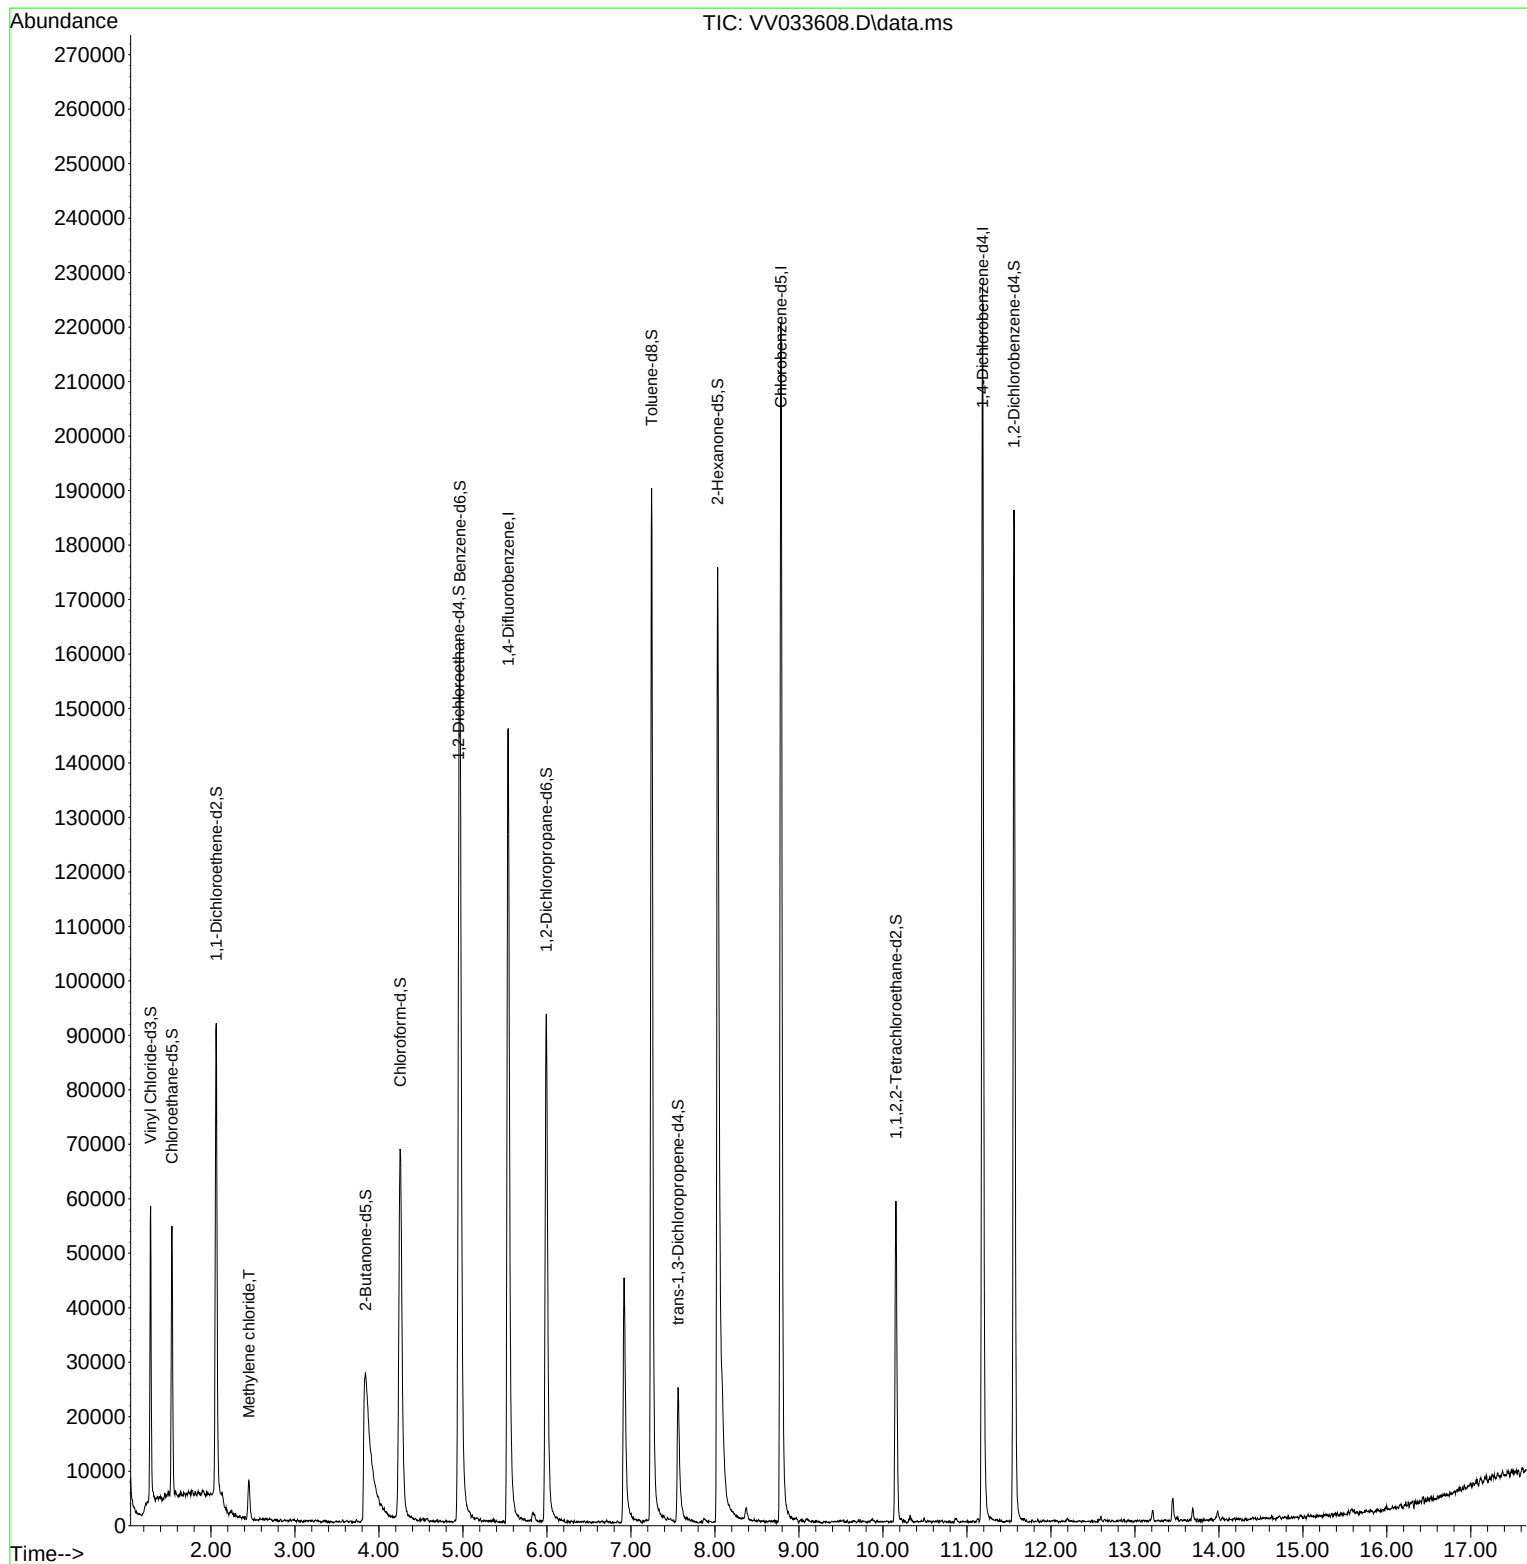

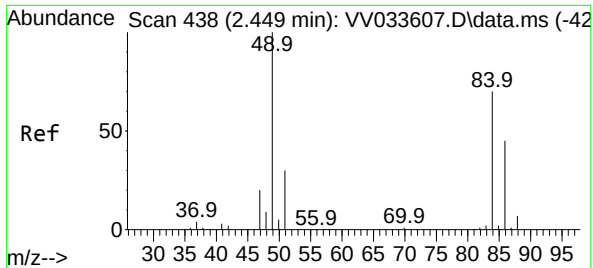

#16
Methylene chloride
Concen: 0.263 ug/L
RT: 2.452 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV033608.D
Acq: 12 Jan 2024 20:42

Instrument :
MSVOA_V
ClientSampleId :
VBLK392

Tgt Ion:	84	Resp:	2786
Ion	Ratio	Lower	Upper
84	100		
86	66.5	45.5	84.5
49	144.5	100.3	186.3

