

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
 Data File : VV033600.D
 Acq On : 12 Jan 2024 17:08
 Operator : SY/MD
 Sample : P1108-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV033600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.086	10	14	24	rVB	11687	11912	2.72%	0.338%
2	1.278	67	74	85	rBV	54517	57988	13.26%	1.645%
3	1.532	146	153	166	rVB	46059	54763	12.52%	1.554%
4	2.060	308	317	331	rVB	86558	124140	28.39%	3.522%
5	3.835	858	869	905	rBV2	25171	110818	25.34%	3.144%
6	4.253	984	999	1026	rBV2	65239	172598	39.47%	4.897%
7	4.960	1205	1219	1250	rBV2	155089	394916	90.32%	11.205%
8	5.535	1386	1398	1424	rBV	146148	308773	70.61%	8.761%
9	5.992	1527	1540	1566	rBV	90584	194491	44.48%	5.519%
10	6.918	1816	1828	1856	rBV2	42915	88215	20.17%	2.503%
11	7.246	1920	1930	1951	rBV	181781	329771	75.42%	9.357%
12	7.561	2018	2028	2043	rBV2	23883	45798	10.47%	1.299%
13	8.034	2165	2175	2217	rBV	158988	395514	90.45%	11.222%
14	8.786	2398	2409	2438	rBV2	223026	437265	100.00%	12.407%
15	10.156	2823	2835	2858	rVB	56745	94614	21.64%	2.685%
16	10.323	2880	2887	2897	rBV3	3220	5331	1.22%	0.151%
17	10.998	3089	3097	3105	rBV4	3102	5322	1.22%	0.151%
18	11.130	3131	3138	3146	rBV5	2920	5631	1.29%	0.160%
19	11.188	3146	3156	3177	rVB	234631	380140	86.94%	10.786%
20	11.561	3258	3272	3291	rBV	187111	301851	69.03%	8.565%
21	13.989	4019	4027	4035	rVB3	2401	4482	1.03%	0.127%




Sum of corrected areas: 3524333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033600.D
Acq On : 12 Jan 2024 17:08
Operator : SY/MD
Sample : P1108-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

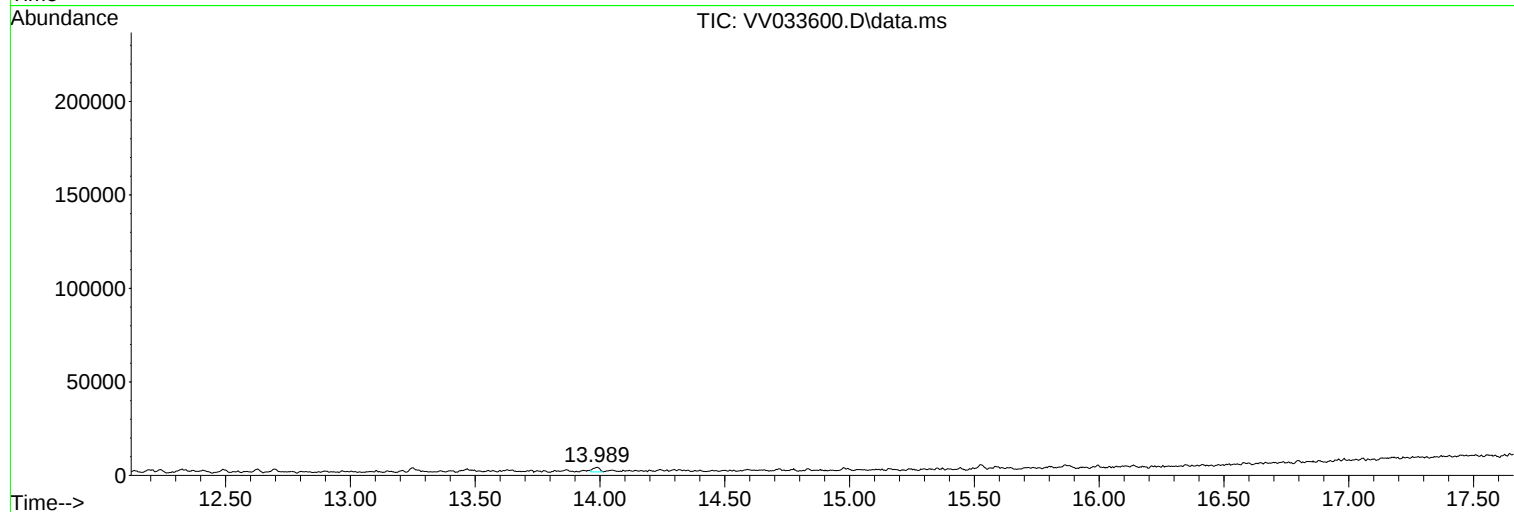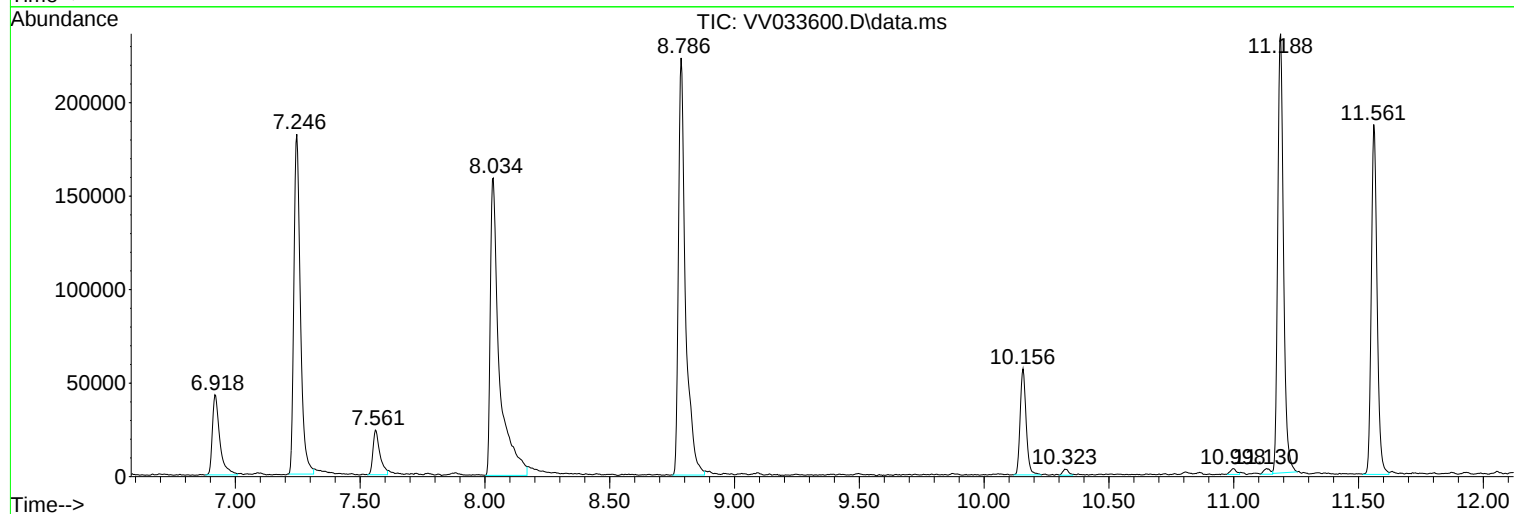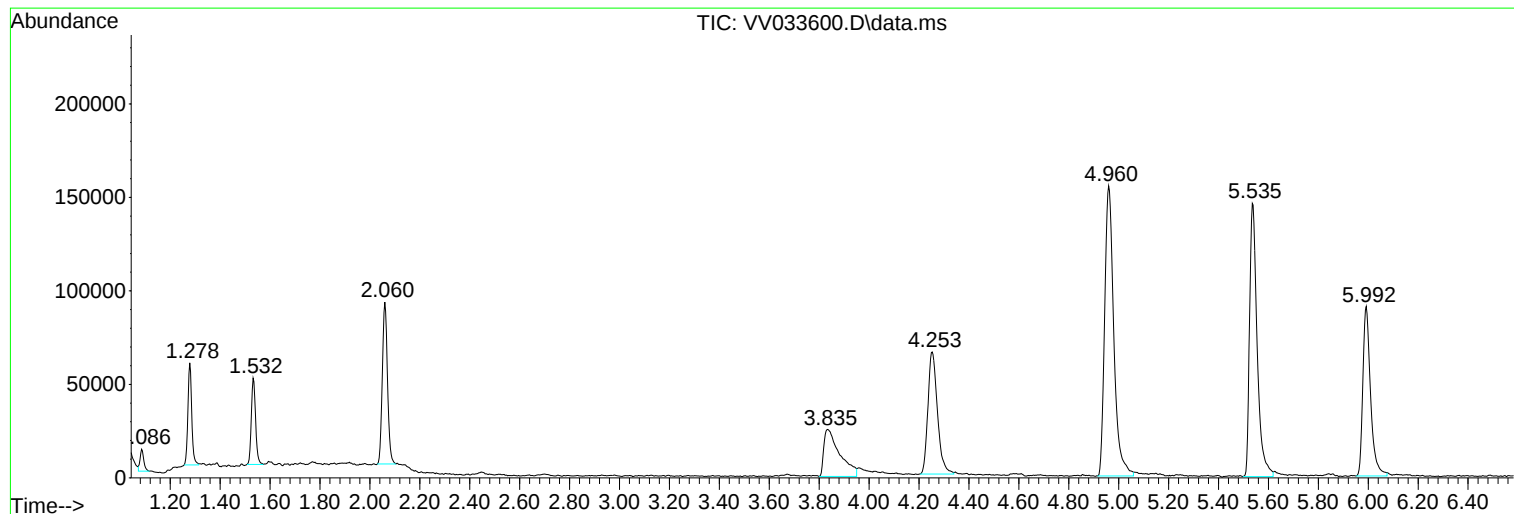

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033600.D
Acq On : 12 Jan 2024 17:08
Operator : SY/MD
Sample : P1108-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033600.D
Acq On : 12 Jan 2024 17:08
Operator : SY/MD
Sample : P1108-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc