

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
 Data File : VV033601.D
 Acq On : 12 Jan 2024 17:31
 Operator : SY/MD
 Sample : P1108-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV033601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	59	rBV	4146	4465	1.07%	0.122%
2	1.281	68	75	87	rBV	55272	57190	13.70%	1.569%
3	1.535	147	154	164	rVB	48025	55970	13.41%	1.535%
4	2.063	307	318	330	rBV	88761	132780	31.81%	3.642%
5	3.805	850	860	905	rBV2	50223	171444	41.08%	4.703%
6	4.252	982	999	1033	rBV	69379	185240	44.38%	5.081%
7	4.960	1204	1219	1245	rBV2	161955	414134	99.22%	11.360%
8	5.539	1388	1399	1424	rBV	143117	300476	71.99%	8.242%
9	5.844	1484	1494	1513	rBV5	13314	30482	7.30%	0.836%
10	5.992	1527	1540	1564	rBV	95233	200625	48.07%	5.503%
11	6.918	1816	1828	1854	rBV	44991	92727	22.22%	2.544%
12	7.246	1919	1930	1950	rBV	192492	348437	83.48%	9.558%
13	7.561	2017	2028	2044	rBV	24686	49131	11.77%	1.348%
14	8.027	2159	2173	2220	rBV	188551	417384	100.00%	11.449%
15	8.786	2399	2409	2430	rBV	220735	383342	91.84%	10.515%
16	9.085	2493	2502	2520	rBV2	6250	11947	2.86%	0.328%
17	10.156	2822	2835	2853	rBV	59777	96148	23.04%	2.637%
18	10.394	2902	2909	2914	rBV3	2704	4389	1.05%	0.120%
19	10.857	3045	3053	3066	rBV2	5927	9348	2.24%	0.256%
20	11.185	3146	3155	3175	rVB	229342	364459	87.32%	9.997%
21	11.561	3259	3272	3290	rBV	191500	315477	75.58%	8.654%




Sum of corrected areas: 3645595

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033601.D
Acq On : 12 Jan 2024 17:31
Operator : SY/MD
Sample : P1108-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

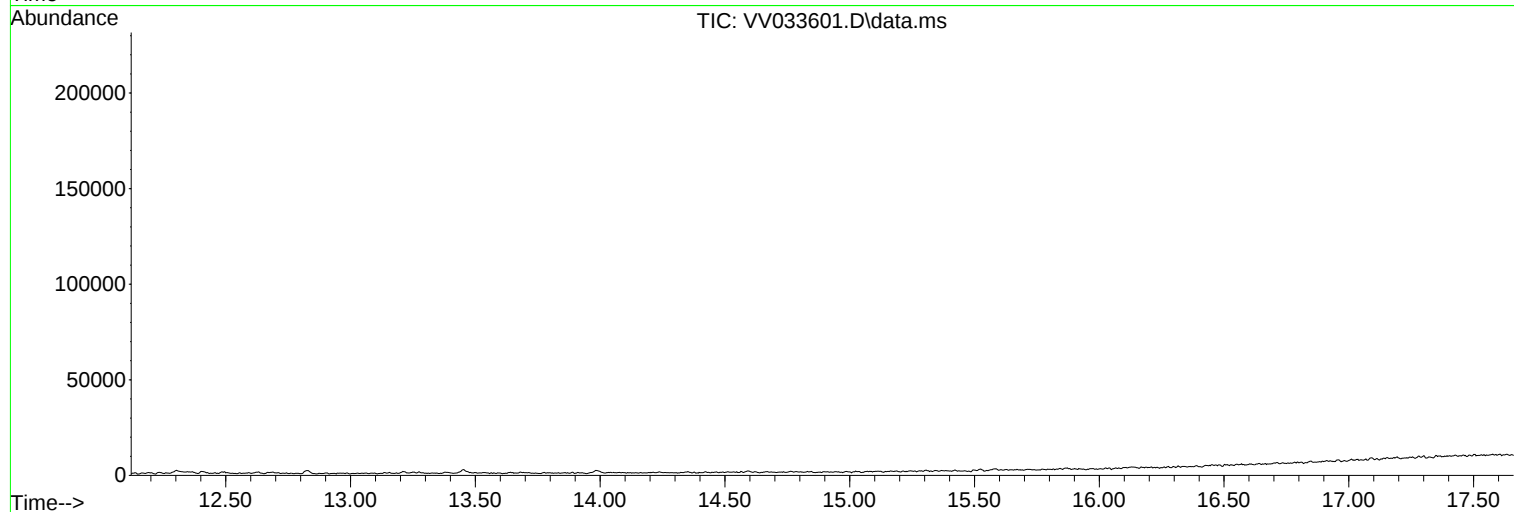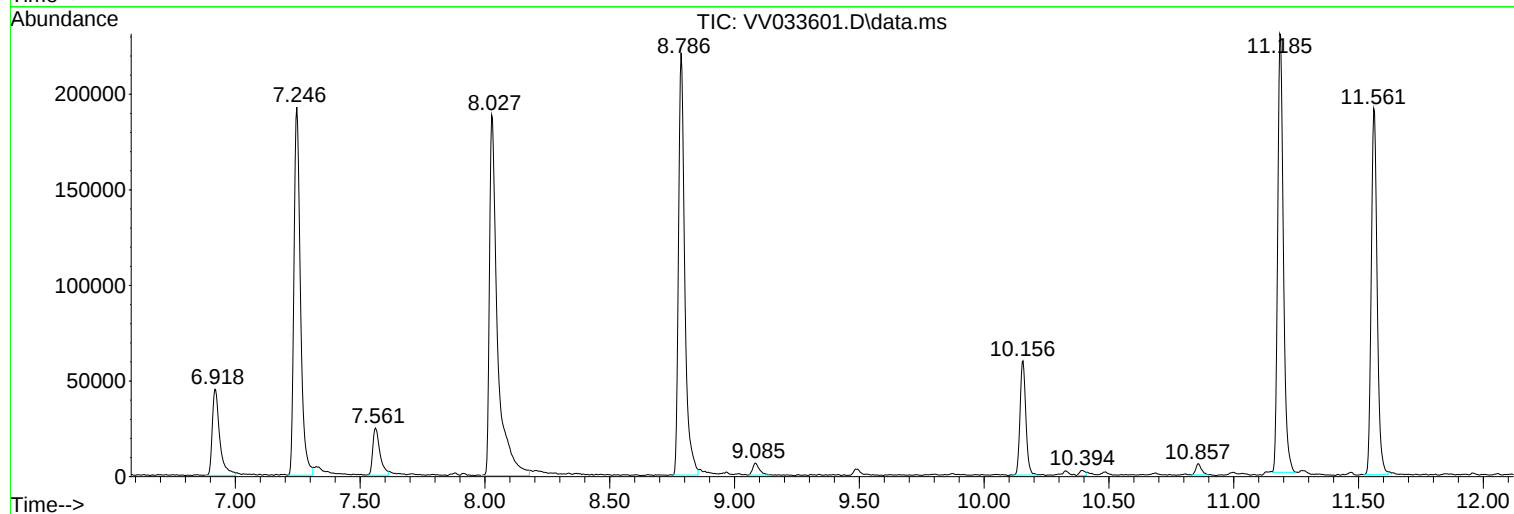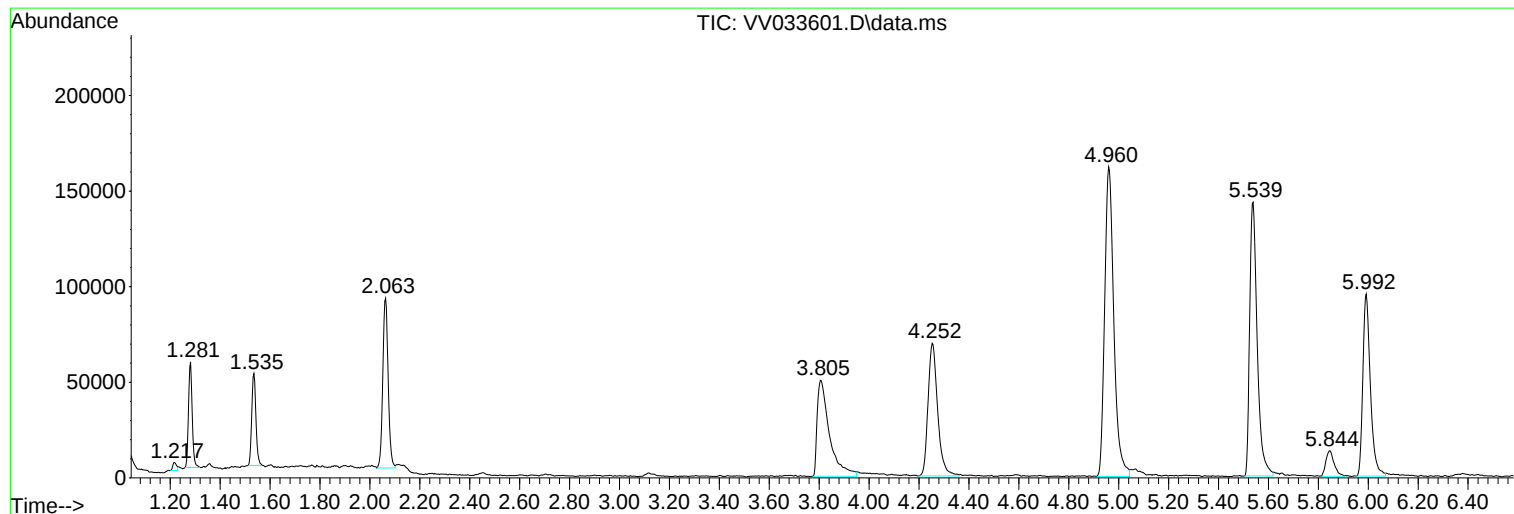

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033601.D
Acq On : 12 Jan 2024 17:31
Operator : SY/MD
Sample : P1108-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033601.D
Acq On : 12 Jan 2024 17:31
Operator : SY/MD
Sample : P1108-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc