
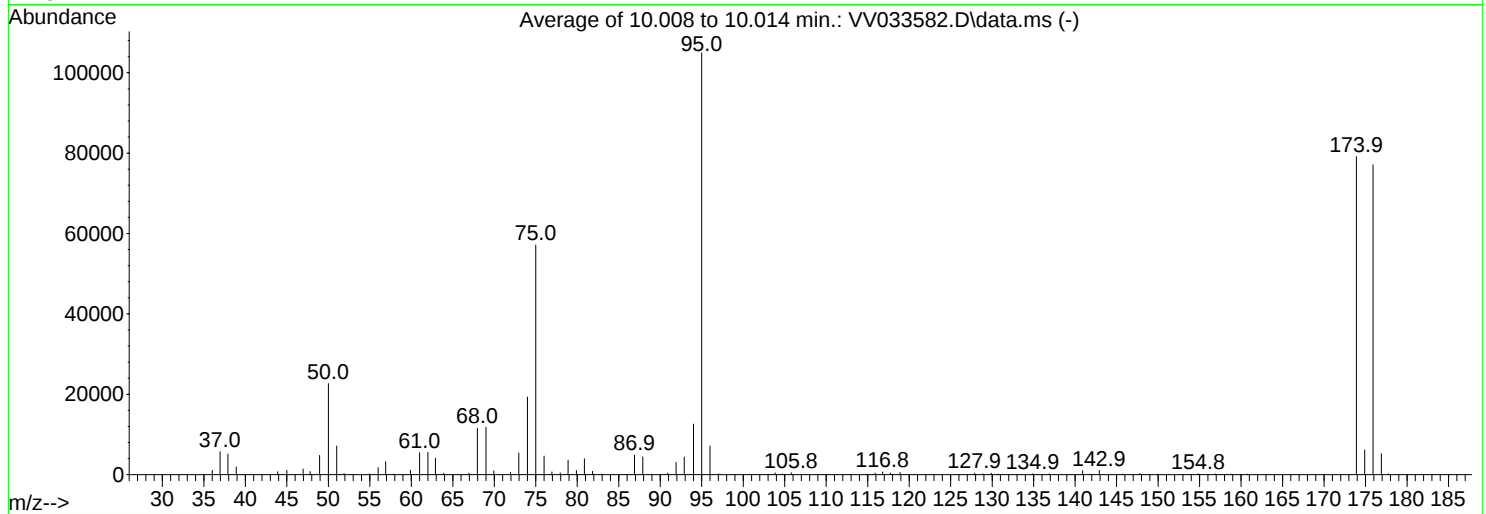


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011224\
Data File : VV033582.D
Acq On : 12 Jan 2024 08:44
Operator : SY/MD
Sample : BFB237
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB237

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jan 13 00:29:44 2024

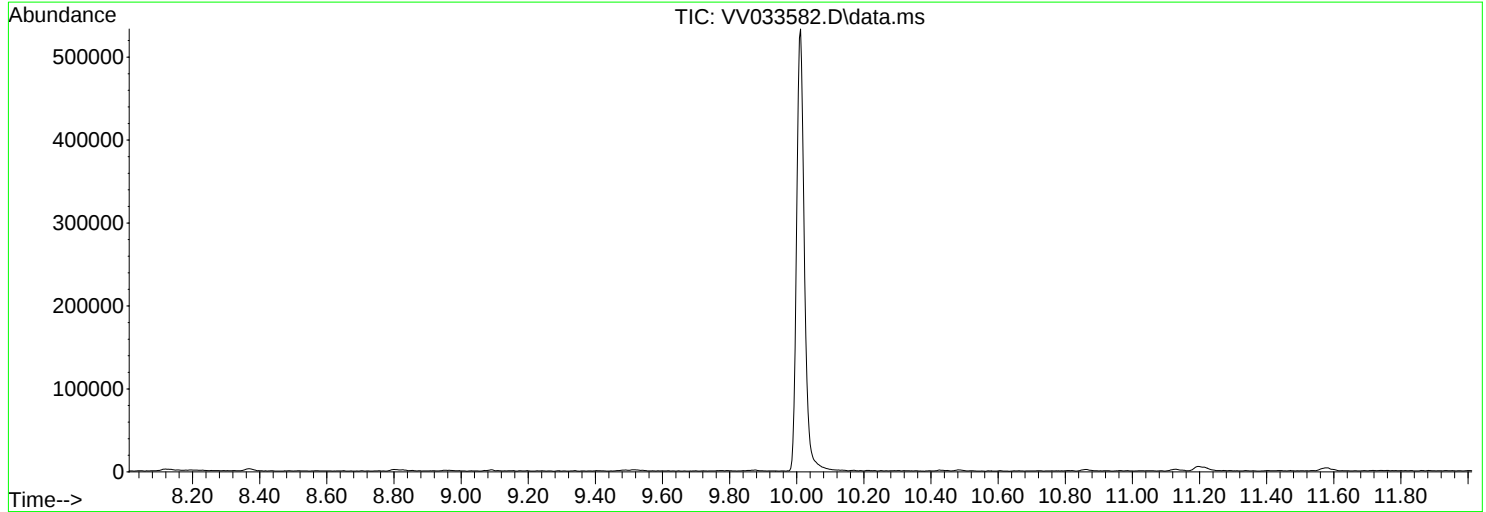

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	22667	PASS
75	95	30	80	54.5	57147	PASS
95	95	100	100	100.0	104949	PASS
96	95	5	9	6.8	7138	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.4	79139	PASS
175	174	5	9	7.8	6149	PASS
176	174	95	105	97.5	77131	PASS
177	176	5	10	6.7	5198	PASS

m/z	Abundance
38.90	127.0
39.80	140.0
41.00	165.0
43.00	200.0
43.90	282.0
55.00	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
36.00	1068.0
36.90	5867.0
37.90	5220.0
38.90	2100.0
39.90	225.0
40.90	276.0
42.90	245.0
43.90	1022.0
45.00	1073.0
46.90	1450.0
47.80	713.0
49.00	4962.0
50.00	23312.0
51.00	7473.0
51.90	324.0
54.90	394.0
56.00	1864.0
56.90	3337.0
57.90	167.0
59.90	1175.0
61.00	5730.0
62.00	5501.0
62.90	4239.0
63.90	382.0
66.90	399.0
68.00	11682.0
69.00	11864.0
70.00	1056.0
72.00	612.0
72.90	5535.0
74.00	19600.0
75.00	58144.0
76.00	4722.0
76.90	635.0
77.90	454.0
78.90	3812.0
79.90	1080.0
80.90	4029.0
81.80	841.0
82.90	147.0
86.90	4902.0
87.90	4328.0
90.90	429.0
91.90	3035.0
92.90	4474.0
94.00	12894.0
95.00	107448.0
96.00	7336.0
97.00	210.0
103.90	429.0
104.80	165.0
105.80	476.0
106.90	103.0
112.90	161.0
114.80	103.0
115.90	418.0
116.80	718.0
117.80	367.0
118.90	534.0
127.90	388.0
128.90	197.0
129.90	358.0
130.80	118.0
134.90	244.0
136.90	220.0
140.90	1017.0
141.80	110.0
142.90	1040.0
145.70	138.0
147.80	282.0
149.90	135.0
153.90	106.0
154.90	215.0
156.90	211.0
158.80	116.0
160.80	112.0
173.90	78968.0
174.90	6080.0
175.90	76064.0
176.90	5331.0
177.80	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
36.00	1082.0
36.90	5894.0
37.90	5256.0
38.90	2139.0
39.90	199.0
41.00	279.0
42.90	248.0
43.90	1040.0
45.00	1094.0
47.00	1414.0
47.80	763.0
49.00	4927.0
50.00	23432.0
51.00	7325.0
51.90	304.0
54.90	362.0
56.00	1839.0
56.90	3397.0
57.90	144.0
59.90	1091.0
61.00	5586.0
62.00	5751.0
62.90	4277.0
63.90	347.0
67.00	406.0
68.00	11916.0
69.00	12150.0
70.00	999.0
70.90	118.0
71.90	596.0
73.00	5631.0
74.00	19896.0
75.00	59136.0
76.00	4795.0
77.00	690.0
78.00	462.0
78.90	3750.0
79.90	1090.0
80.90	4077.0
81.80	860.0
82.90	148.0
86.00	127.0
86.90	5028.0
87.90	4653.0
90.90	407.0
91.90	3121.0
92.90	4534.0
94.00	12954.0
95.00	108360.0
96.00	7404.0
97.10	203.0
103.80	454.0
104.70	168.0
105.80	514.0
111.00	102.0
112.90	131.0
114.80	110.0
115.90	387.0
116.80	695.0
117.80	361.0
118.90	566.0
127.90	392.0
128.90	201.0
129.90	384.0
130.70	124.0
134.90	257.0
136.90	206.0
140.90	1005.0
141.80	102.0
142.90	1079.0
144.90	107.0
145.70	152.0
147.80	276.0
150.00	145.0
154.80	235.0
156.90	230.0
158.80	110.0
160.70	122.0
173.90	81776.0
174.90	6391.0
175.90	79864.0
176.90	5374.0
177.80	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237

m/z	Abundance
36.00	1062.0
37.00	5301.0
37.90	4793.0
38.90	1938.0
39.90	182.0
41.00	222.0
43.00	224.0
43.90	965.0
45.00	1045.0
47.00	1284.0
47.80	766.0
48.90	4437.0
50.00	21256.0
51.00	6616.0
51.90	238.0
55.00	342.0
56.00	1616.0
56.90	3101.0
57.90	108.0
59.90	922.0
61.00	5022.0
62.00	5298.0
62.90	3781.0
63.90	352.0
67.00	370.0
67.90	10981.0
69.00	11368.0
69.90	839.0
70.90	105.0
71.90	576.0
73.00	4976.0
74.00	18424.0
75.00	54160.0
76.00	4333.0
77.00	690.0
78.00	446.0
78.90	3323.0
79.90	979.0
80.80	3691.0
81.90	807.0
83.00	136.0
85.90	160.0
86.90	4610.0
87.90	4328.0
90.90	376.0
91.90	2979.0
92.90	4201.0
94.00	11920.0
95.00	99040.0
96.00	6675.0
97.00	192.0
103.80	447.0
104.80	159.0
105.80	493.0
109.60	106.0
110.80	110.0
114.80	109.0
115.90	352.0
116.80	653.0
117.70	317.0
118.90	534.0
127.90	334.0
128.90	176.0
129.90	369.0
130.70	124.0
134.90	235.0
136.90	174.0
140.90	924.0
141.70	107.0
142.90	1003.0
145.00	108.0
145.70	131.0
147.80	282.0
150.00	128.0
154.80	226.0
156.90	210.0
158.80	101.0
160.70	125.0
173.90	76672.0
174.90	5976.0
175.90	75464.0
176.90	4888.0
177.80	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB237