

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029846.D
 Acq On : 14 Jan 2023 09:59
 Operator : SY/MD
 Sample : VV0113WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK291

Quant Time: Jan 16 00:39:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 12 22:05:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.603	114	219285	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	211631	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	110007	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	84786	5.098	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.000%
7) Chloroethane-d5	1.564	69	72892	5.287	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.800%
11) 1,1-Dichloroethene-d2	2.101	63	111896	3.690	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.800%
20) 2-Butanone-d5	3.908	46	134085	45.483	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.960%
24) Chloroform-d	4.333	84	151049	4.951	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	5.021	65	65284	5.052	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%
32) Benzene-d6	5.037	84	319142	5.084	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	6.056	67	94719	5.156	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.200%
41) Toluene-d8	7.304	98	275020	4.732	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
43) trans-1,3-Dichloroprop...	7.612	79	28450	4.240	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.800%
46) 2-Hexanone-d5	8.085	63	130937	47.932	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.860%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	68380	5.079	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.600%
66) 1,2-Dichlorobenzene-d4	11.612	152	101792	5.090	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.800%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	10185	0.438	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029846.D
Acq On : 14 Jan 2023 09:59
Operator : SY/MD
Sample : VV0113WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK291


Quant Time: Jan 16 00:39:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 12 22:05:54 2023
Response via : Initial Calibration

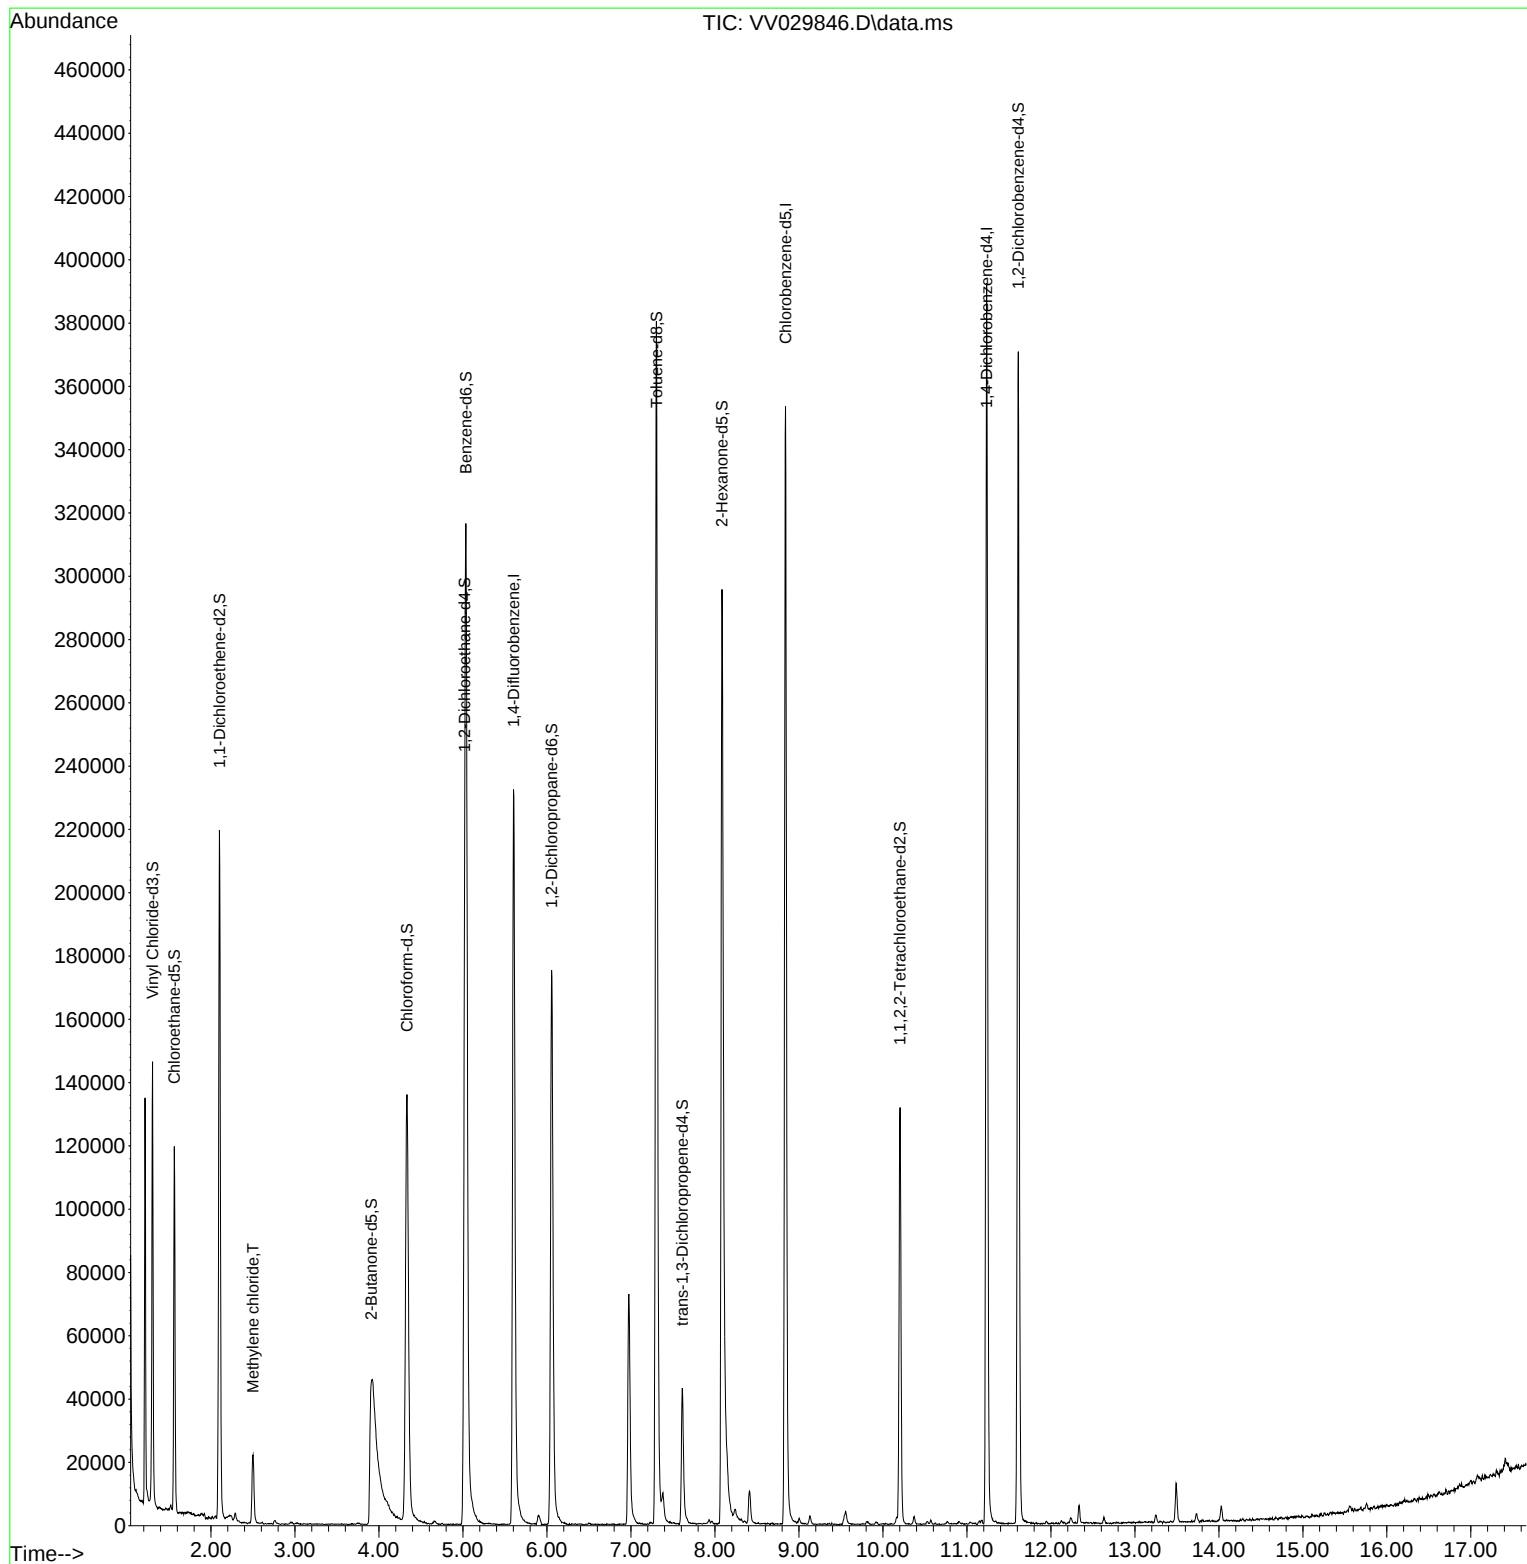

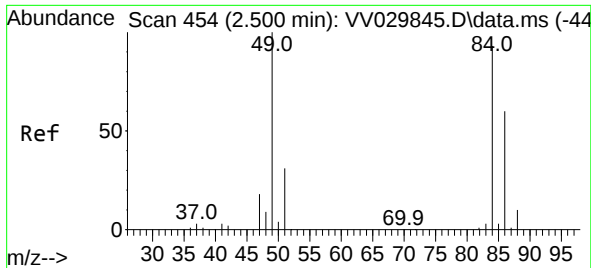

#16
Methylene chloride
Concen: 0.438 ug/L
RT: 2.500 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV029846.D
Acq: 14 Jan 2023 09:59

Instrument :
MSVOA_V
ClientSampleId :
VBLK291

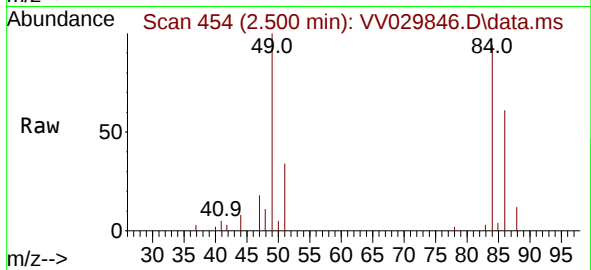

Tgt Ion: 84 Resp: 10185
Ion Ratio Lower Upper
84 100
86 64.9 45.0 83.6
49 106.2 71.5 132.7

