

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029809.D
 Acq On : 13 Jan 2023 15:31
 Operator : SY/MD
 Sample : 01138-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1W5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029809.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB2	147514	161400	14.21%	2.150%
2	1.565	156	163	179	rVB	103259	115292	10.15%	1.536%
3	1.802	230	237	249	rVB	20154	26627	2.34%	0.355%
4	2.105	319	331	346	rBV2	201915	303849	26.75%	4.048%
5	3.185	656	667	681	rVB2	8261	16964	1.49%	0.226%
6	3.902	874	890	927	rBV2	216226	634719	55.88%	8.455%
7	4.339	1006	1026	1049	rBV	126891	317530	27.95%	4.230%
8	5.040	1226	1244	1278	rBV2	291786	745430	65.63%	9.930%
9	5.609	1408	1421	1443	rBV	212901	434988	38.30%	5.795%
10	5.905	1499	1513	1546	rBV	569517	1135876	100.00%	15.132%
11	6.063	1548	1562	1584	rVV	166591	343338	30.23%	4.574%
12	6.979	1836	1847	1874	rBV	70279	134049	11.80%	1.786%
13	7.307	1937	1949	1969	rBV	355400	642239	56.54%	8.556%
14	7.616	2034	2045	2064	rBV	39504	70419	6.20%	0.938%
15	8.085	2181	2191	2227	rBV	282403	552207	48.62%	7.356%
16	8.844	2414	2427	2449	rBV	322759	536472	47.23%	7.147%
17	10.207	2840	2851	2865	rVB	123758	198040	17.44%	2.638%
18	11.236	3160	3171	3193	rBV	360930	560484	49.34%	7.467%
19	11.612	3277	3288	3317	rVB	362708	576688	50.77%	7.682%




Sum of corrected areas: 7506611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029809.D
Acq On : 13 Jan 2023 15:31
Operator : SY/MD
Sample : 01138-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

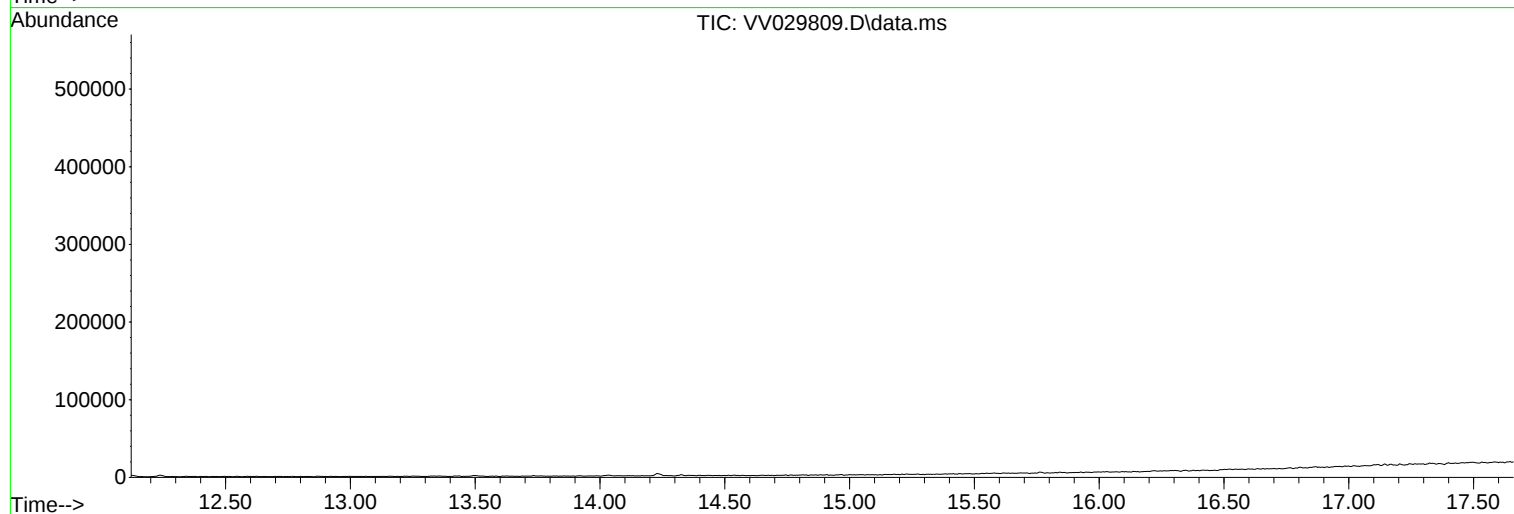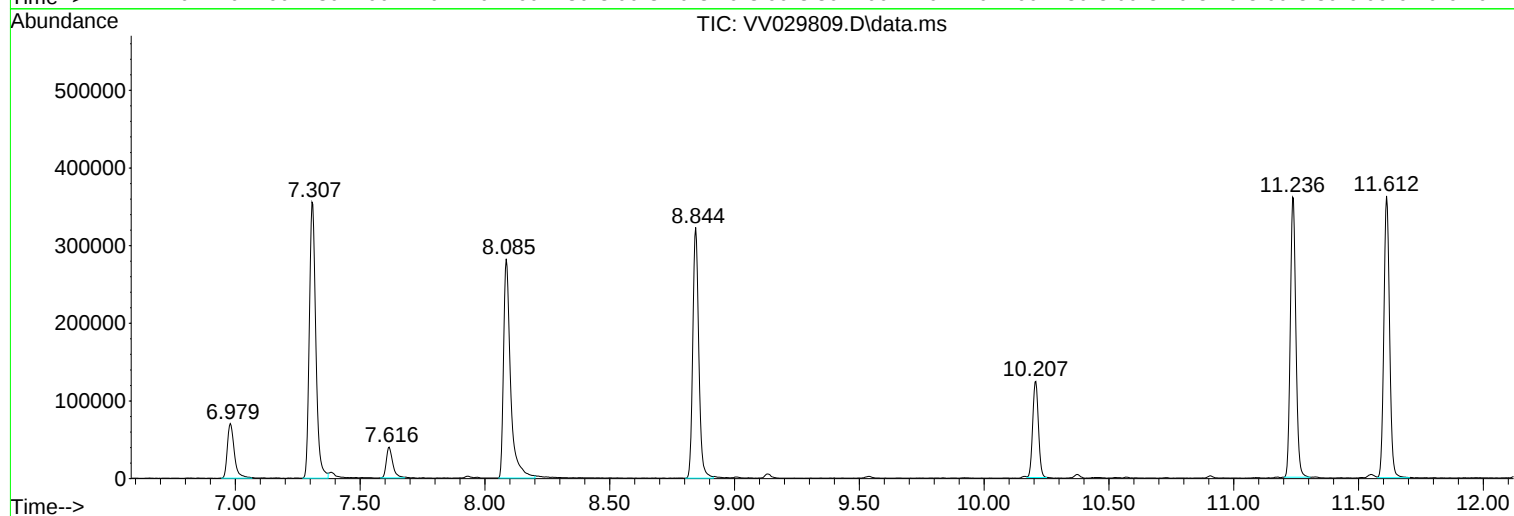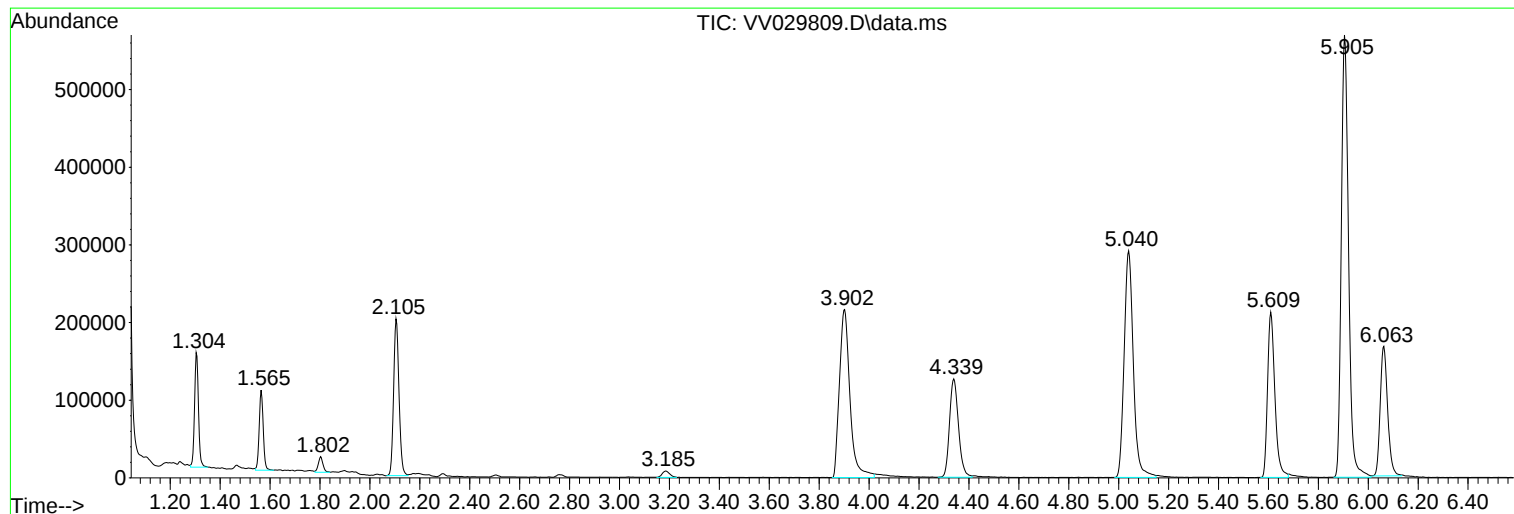

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029809.D
Acq On : 13 Jan 2023 15:31
Operator : SY/MD
Sample : 01138-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029809.D
Acq On : 13 Jan 2023 15:31
Operator : SY/MD
Sample : 01138-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc