

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029814.D
 Acq On : 13 Jan 2023 17:29
 Operator : SY/MD
 Sample : 01138-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1X1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	119181	118879	15.74%	1.633%
2	1.564	155	163	175	rVB	105349	116371	15.41%	1.598%
3	2.105	321	331	346	rBV2	200233	306832	40.63%	4.215%
4	2.359	394	410	411	rBV2	4964	10123	1.34%	0.139%
5	2.764	520	536	560	rBV	264644	556665	73.70%	7.646%
6	3.182	655	666	688	rVB2	6849	15092	2.00%	0.207%
7	3.886	875	885	937	rBV	70073	241515	31.98%	3.317%
8	4.339	1006	1026	1053	rBV	131302	335318	44.40%	4.606%
9	4.596	1095	1106	1121	rBV6	4569	11057	1.46%	0.152%
10	5.040	1224	1244	1269	rBV2	300127	755270	100.00%	10.374%
11	5.609	1408	1421	1444	rBV	205988	425284	56.31%	5.842%
12	5.908	1500	1514	1548	rBV	272355	550873	72.94%	7.567%
13	6.063	1548	1562	1593	rVV	169982	354733	46.97%	4.872%
14	6.979	1831	1847	1872	rBV	74076	141245	18.70%	1.940%
15	7.307	1934	1949	1966	rBV	362755	646457	85.59%	8.879%
16	7.384	1966	1973	1991	rVB	26358	49836	6.60%	0.685%
17	7.616	2036	2045	2063	rBV2	43534	76582	10.14%	1.052%
18	7.966	2148	2154	2165	rVB5	5154	8997	1.19%	0.124%
19	8.085	2180	2191	2234	rBV	330632	636837	84.32%	8.747%
20	8.844	2414	2427	2457	rBV	315965	533966	70.70%	7.334%
21	9.133	2508	2517	2531	rVB2	6530	11052	1.46%	0.152%
22	9.558	2635	2649	2662	rBV4	7798	17783	2.35%	0.244%
23	10.207	2840	2851	2871	rVB	130318	207234	27.44%	2.846%
24	10.371	2894	2902	2914	rVB3	7059	11219	1.49%	0.154%
25	11.236	3160	3171	3193	rBV	356592	558378	73.93%	7.670%
26	11.612	3276	3288	3309	rVB	363658	582756	77.16%	8.005%




Sum of corrected areas: 7280354

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029814.D
Acq On : 13 Jan 2023 17:29
Operator : SY/MD
Sample : 01138-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

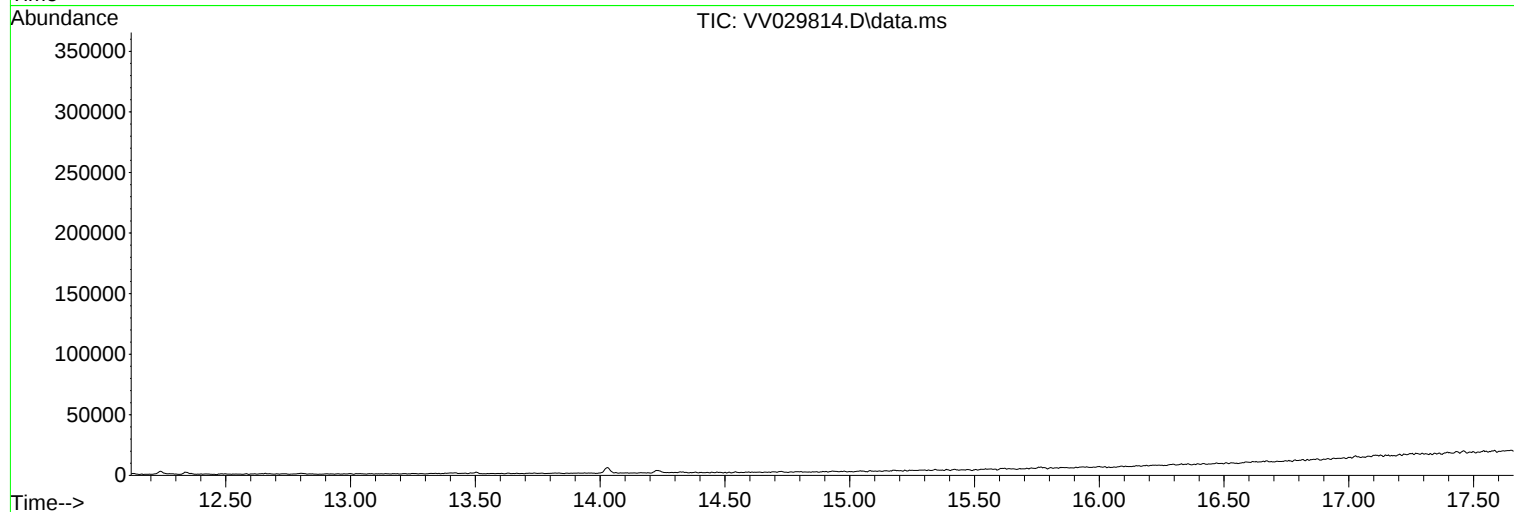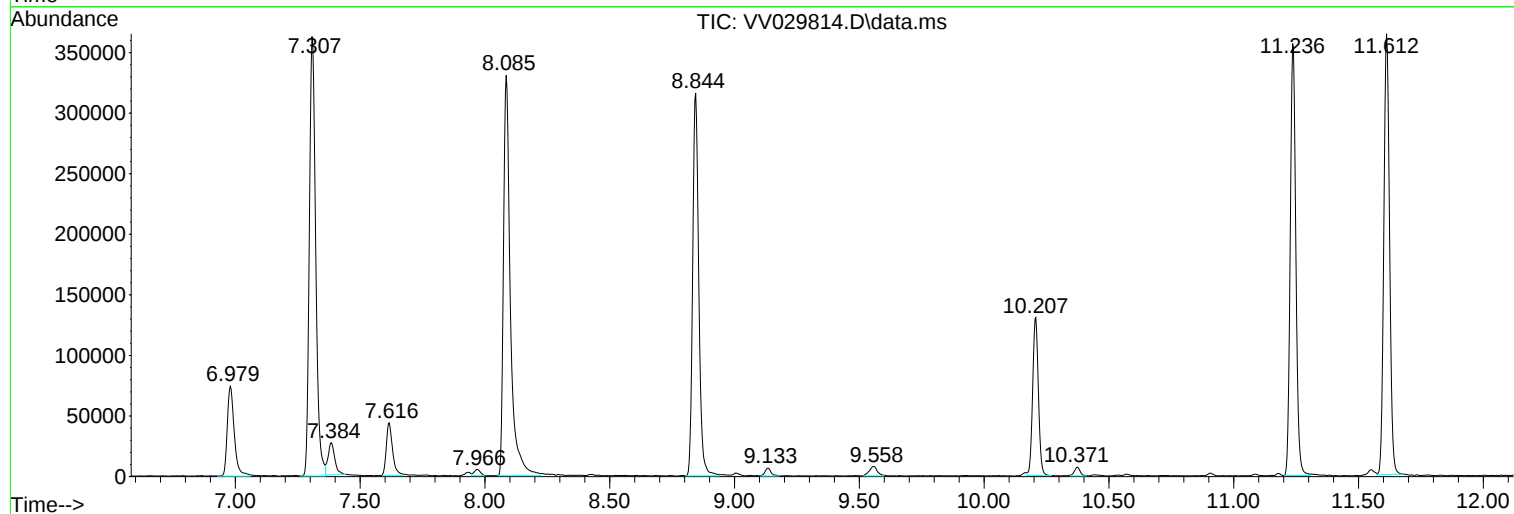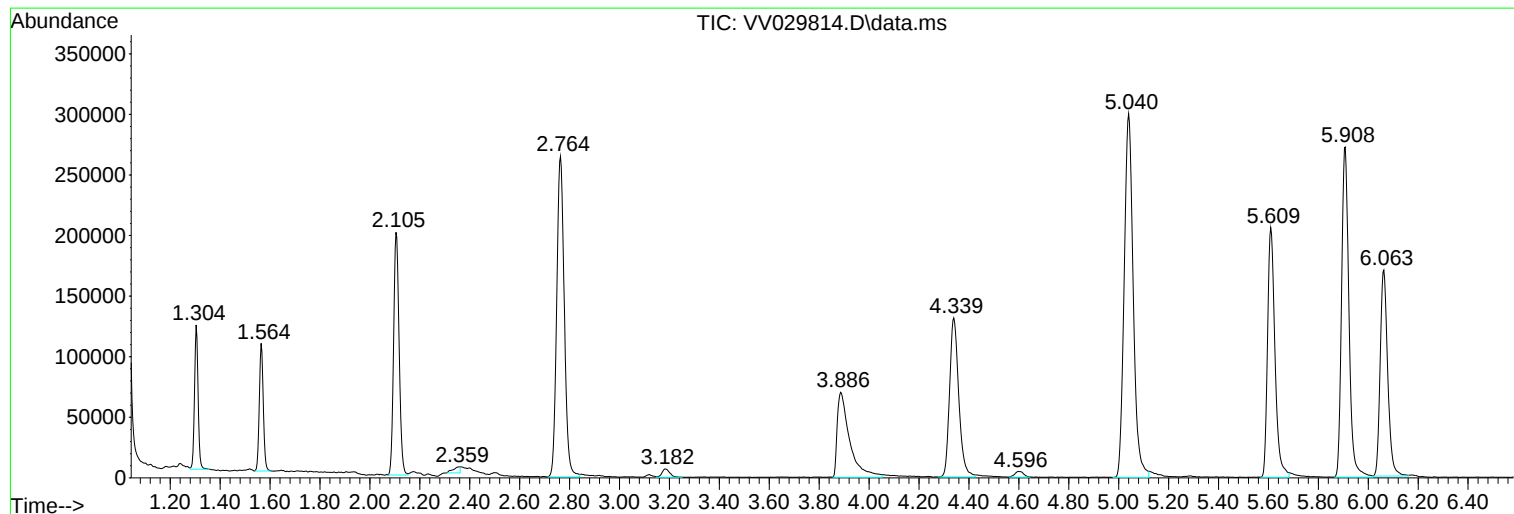

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029814.D
Acq On : 13 Jan 2023 17:29
Operator : SY/MD
Sample : 01138-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029814.D
Acq On : 13 Jan 2023 17:29
Operator : SY/MD
Sample : 01138-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc