

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029816.D
 Acq On : 13 Jan 2023 18:17
 Operator : SY/MD
 Sample : 01138-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1X3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	112	rVB2	164892	203815	27.29%	3.175%
2	1.565	156	163	178	rBV2	107472	148107	19.83%	2.307%
3	1.802	233	237	244	rVB	15154	17723	2.37%	0.276%
4	2.105	322	331	347	rVB2	204686	328410	43.97%	5.116%
5	2.204	355	362	379	rVB2	15376	28518	3.82%	0.444%
6	2.757	523	534	555	rBV	65383	118181	15.82%	1.841%
7	3.185	653	667	686	rBV	42409	90251	12.08%	1.406%
8	3.892	875	887	925	rBV2	61437	212429	28.44%	3.309%
9	4.339	1010	1026	1052	rBV	128131	322850	43.23%	5.029%
10	5.040	1227	1244	1268	rBV2	296659	746819	100.00%	11.634%
11	5.609	1408	1421	1455	rBV	211587	439546	58.86%	6.847%
12	5.912	1502	1515	1535	rBV	38634	79274	10.61%	1.235%
13	6.063	1547	1562	1588	rBV	170541	358488	48.00%	5.585%
14	6.979	1837	1847	1865	rBV	70953	131638	17.63%	2.051%
15	7.307	1936	1949	1966	rBV	366376	647675	86.72%	10.090%
16	7.384	1967	1973	1985	rVB	16415	29264	3.92%	0.456%
17	7.616	2033	2045	2070	rBV	40288	73700	9.87%	1.148%
18	8.085	2181	2191	2225	rBV	249826	497060	66.56%	7.743%
19	8.844	2412	2427	2448	rBV	328059	545905	73.10%	8.504%
20	9.133	2507	2517	2533	rVB2	7780	13513	1.81%	0.211%
21	10.207	2841	2851	2866	rVB	125148	196829	26.36%	3.066%
22	10.374	2887	2903	2913	rBV3	5709	10522	1.41%	0.164%
23	11.236	3159	3171	3196	rVB	368140	579197	77.56%	9.023%
24	11.612	3277	3288	3316	rVB	377189	599581	80.28%	9.340%




Sum of corrected areas: 6419295

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029816.D
Acq On : 13 Jan 2023 18:17
Operator : SY/MD
Sample : 01138-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

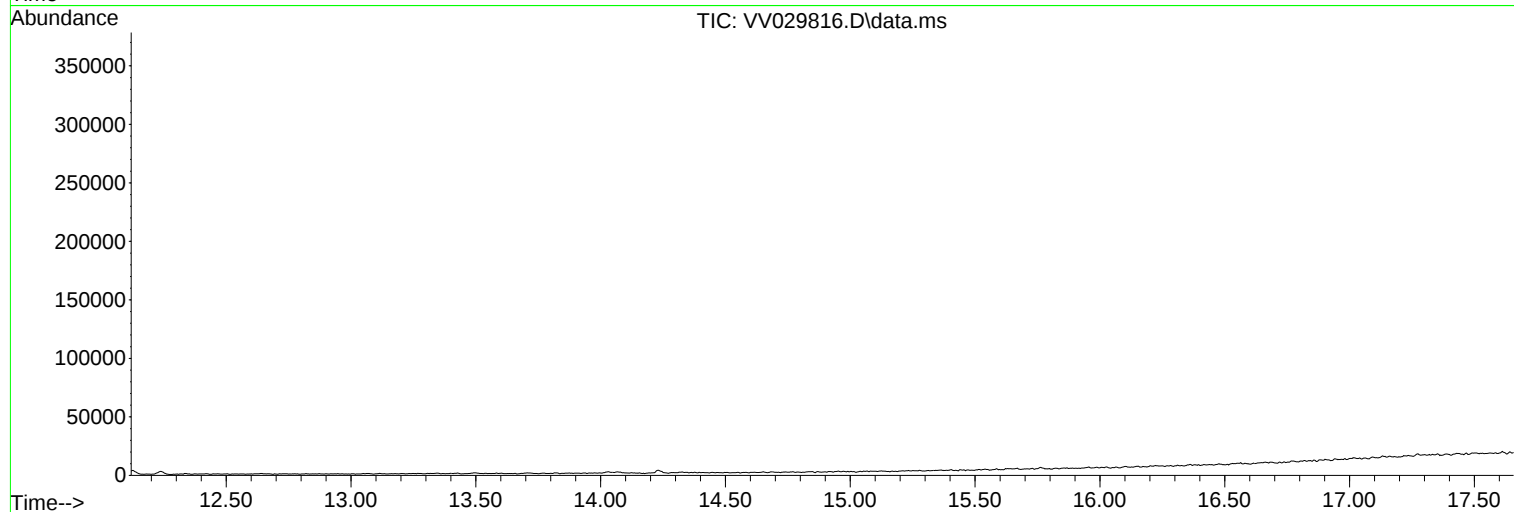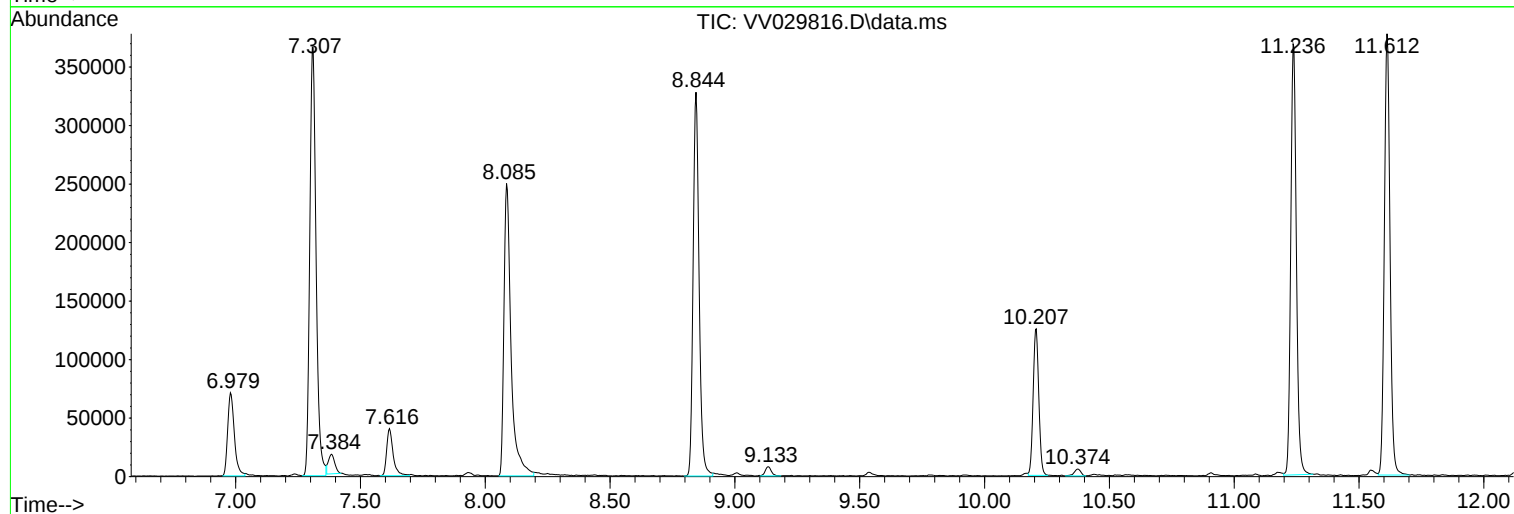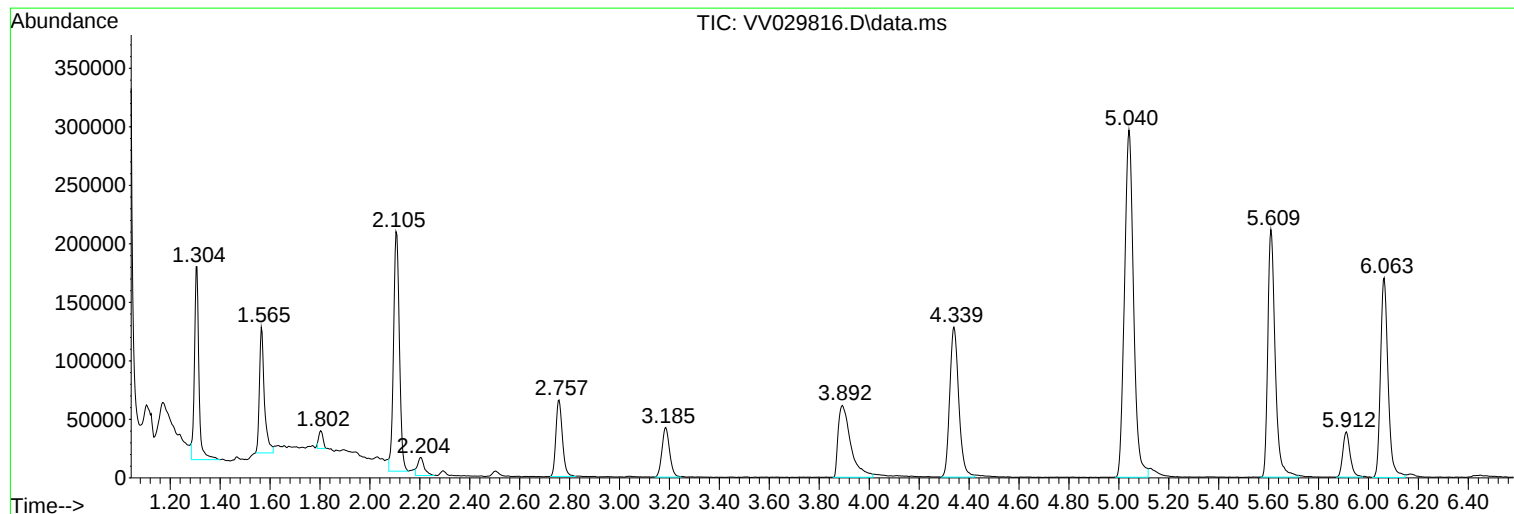

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029816.D
Acq On : 13 Jan 2023 18:17
Operator : SY/MD
Sample : 01138-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029816.D
Acq On : 13 Jan 2023 18:17
Operator : SY/MD
Sample : 01138-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
