

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029817.D
 Acq On : 13 Jan 2023 18:41
 Operator : SY/MD
 Sample : 01138-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1X4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	109095	114901	6.76%	1.433%
2	1.565	156	163	177	rVB	96831	111771	6.57%	1.394%
3	2.114	320	334	352	rBV	1105909	1699965	100.00%	21.208%
4	2.503	445	455	469	rVB2	11539	19495	1.15%	0.243%
5	3.182	649	666	692	rBV	266711	561057	33.00%	6.999%
6	3.886	875	885	934	rBV	72071	249571	14.68%	3.114%
7	4.339	1009	1026	1052	rBV	120517	302607	17.80%	3.775%
8	5.040	1227	1244	1267	rBV3	272583	690620	40.63%	8.616%
9	5.609	1409	1421	1453	rBV	209215	441795	25.99%	5.512%
10	5.908	1501	1514	1538	rBV2	89104	182109	10.71%	2.272%
11	6.063	1549	1562	1583	rBV	157534	329817	19.40%	4.115%
12	6.169	1584	1595	1611	rVB3	19834	42397	2.49%	0.529%
13	6.979	1833	1847	1870	rBV	66248	124891	7.35%	1.558%
14	7.307	1937	1949	1968	rBV	335432	596283	35.08%	7.439%
15	7.616	2032	2045	2066	rBV	37068	68867	4.05%	0.859%
16	8.085	2180	2191	2231	rBV	311819	607037	35.71%	7.573%
17	8.844	2410	2427	2465	rBV	332058	553199	32.54%	6.901%
18	10.204	2840	2850	2871	rVB	121088	195395	11.49%	2.438%
19	11.236	3159	3171	3194	rBV	364452	580979	34.18%	7.248%
20	11.612	3277	3288	3311	rBV	345264	542999	31.94%	6.774%




Sum of corrected areas: 8015755

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029817.D
Acq On : 13 Jan 2023 18:41
Operator : SY/MD
Sample : 01138-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

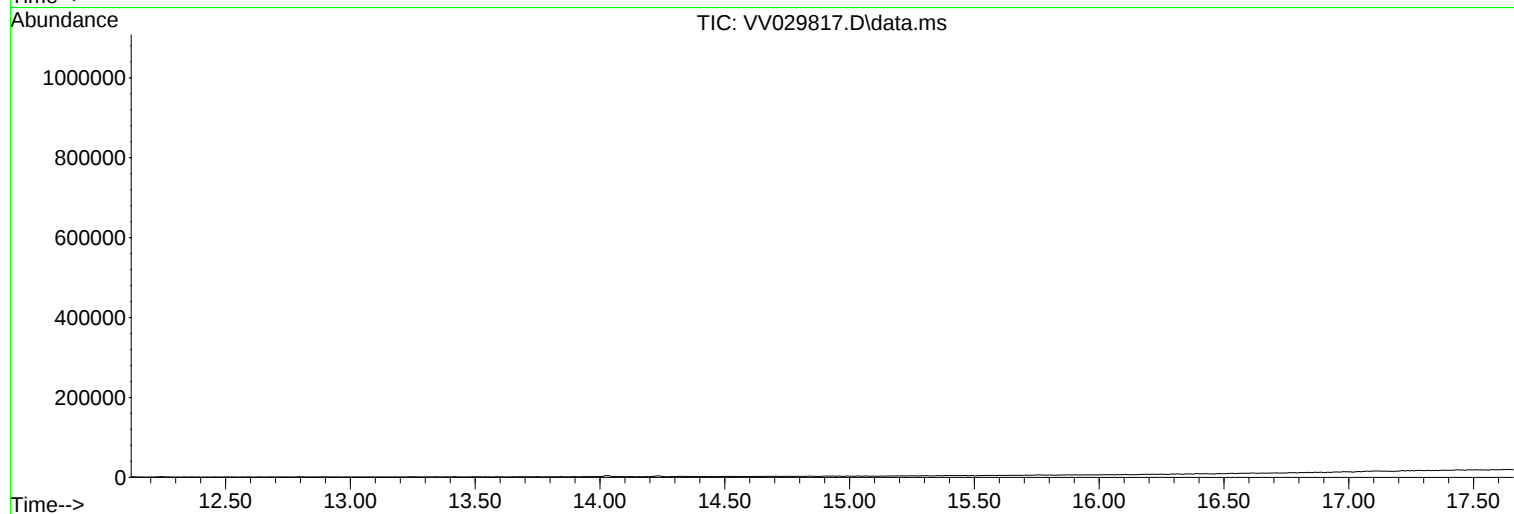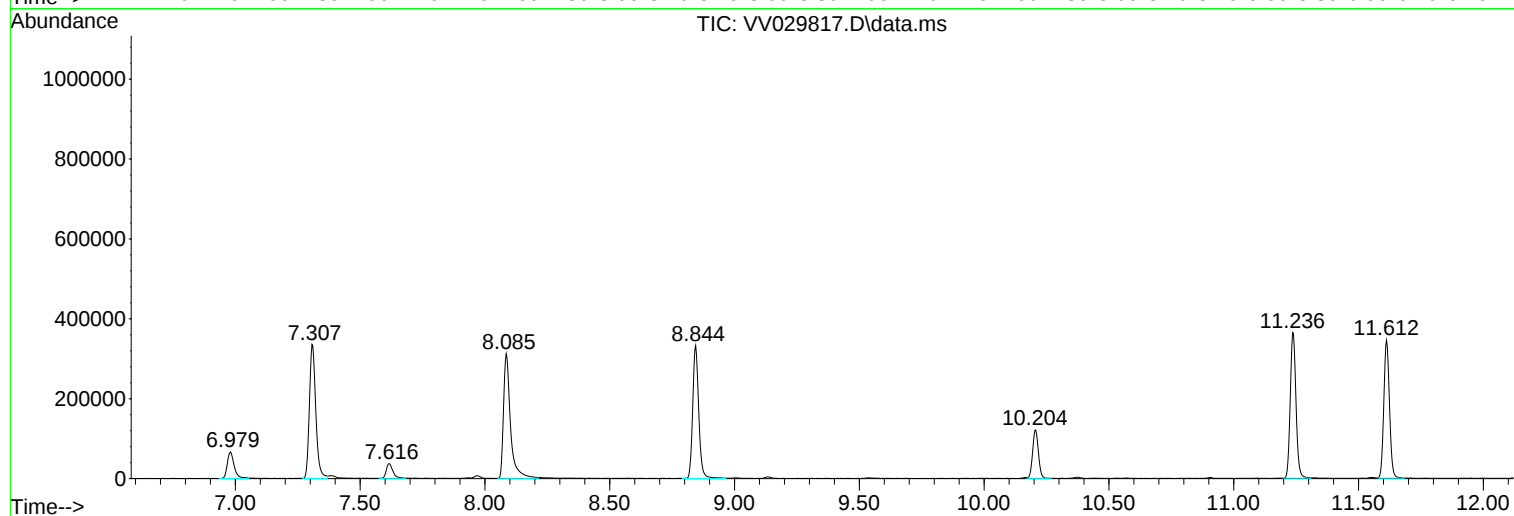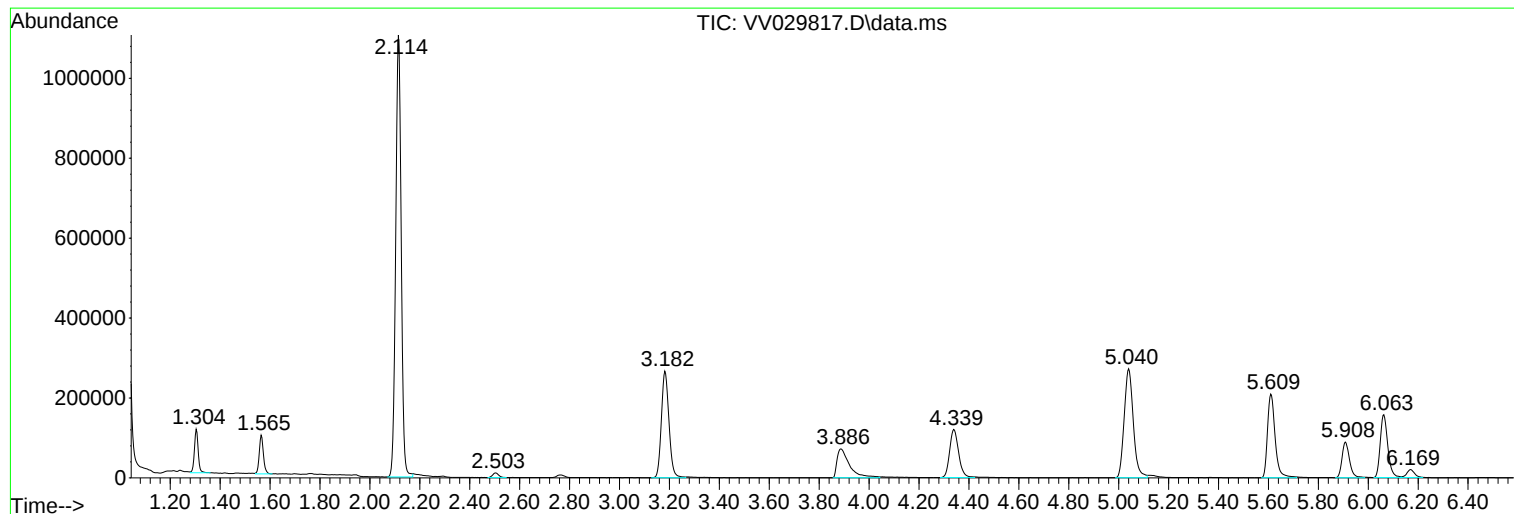

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029817.D
Acq On : 13 Jan 2023 18:41
Operator : SY/MD
Sample : 01138-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029817.D
Acq On : 13 Jan 2023 18:41
Operator : SY/MD
Sample : 01138-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc