

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029848.D
 Acq On : 14 Jan 2023 10:55
 Operator : SY/MD
 Sample : 01149-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0L55

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	95	rVB	114913	117379	16.23%	1.853%
2	1.564	155	163	176	rVB	103674	114929	15.89%	1.814%
3	2.101	320	330	347	rBV	182839	265583	36.72%	4.193%
4	2.767	524	537	553	rVB3	6050	13869	1.92%	0.219%
5	3.899	877	889	942	rBV2	57293	241819	33.43%	3.817%
6	4.339	1008	1026	1046	rBV	123753	308973	42.71%	4.878%
7	4.899	1190	1200	1217	rVB6	3085	7451	1.03%	0.118%
8	5.040	1224	1244	1278	rBV2	281317	723350	100.00%	11.419%
9	5.609	1408	1421	1446	rBV	197696	409829	56.66%	6.470%
10	5.905	1500	1513	1548	rBV2	153567	315833	43.66%	4.986%
11	6.059	1548	1561	1597	rVB	160169	342212	47.31%	5.402%
12	6.979	1835	1847	1874	rBV	70163	134370	18.58%	2.121%
13	7.233	1916	1926	1937	rBV3	4526	9414	1.30%	0.149%
14	7.307	1937	1949	1962	rVV	340098	593314	82.02%	9.366%
15	7.381	1963	1972	1999	rVB	139993	257209	35.56%	4.060%
16	7.616	2035	2045	2070	rBV2	40788	75129	10.39%	1.186%
17	7.931	2134	2143	2155	rBV3	6899	12655	1.75%	0.200%
18	8.085	2180	2191	2227	rBV	304278	604520	83.57%	9.543%
19	8.844	2414	2427	2460	rBV	304288	514040	71.06%	8.115%
20	9.130	2507	2516	2527	rBV3	5551	9368	1.30%	0.148%
21	10.207	2840	2851	2868	rVB	116411	185209	25.60%	2.924%
22	10.374	2889	2903	2913	rBV	18092	28083	3.88%	0.443%
23	11.201	3147	3160	3162	rBV2	10872	13488	1.86%	0.213%
24	11.239	3162	3172	3190	rVB	325855	514410	71.11%	8.121%
25	11.612	3276	3288	3309	rBV	321901	514359	71.11%	8.120%
26	14.030	4031	4040	4048	rBV2	5023	7852	1.09%	0.124%




Sum of corrected areas: 6334647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029848.D
Acq On : 14 Jan 2023 10:55
Operator : SY/MD
Sample : 01149-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

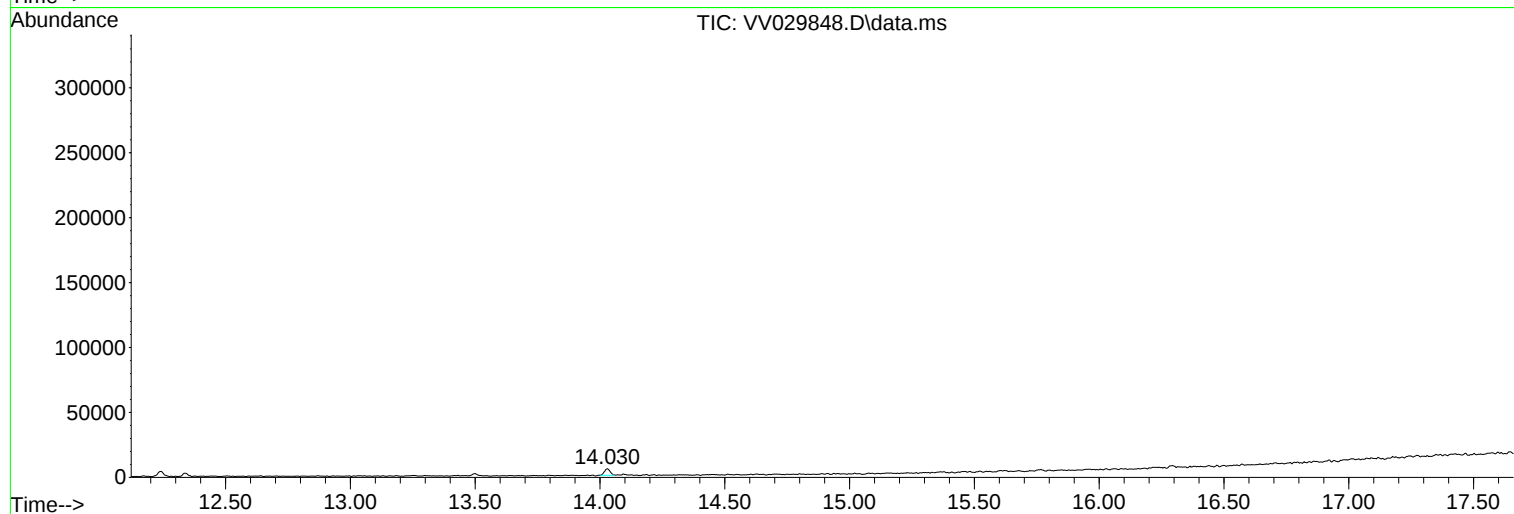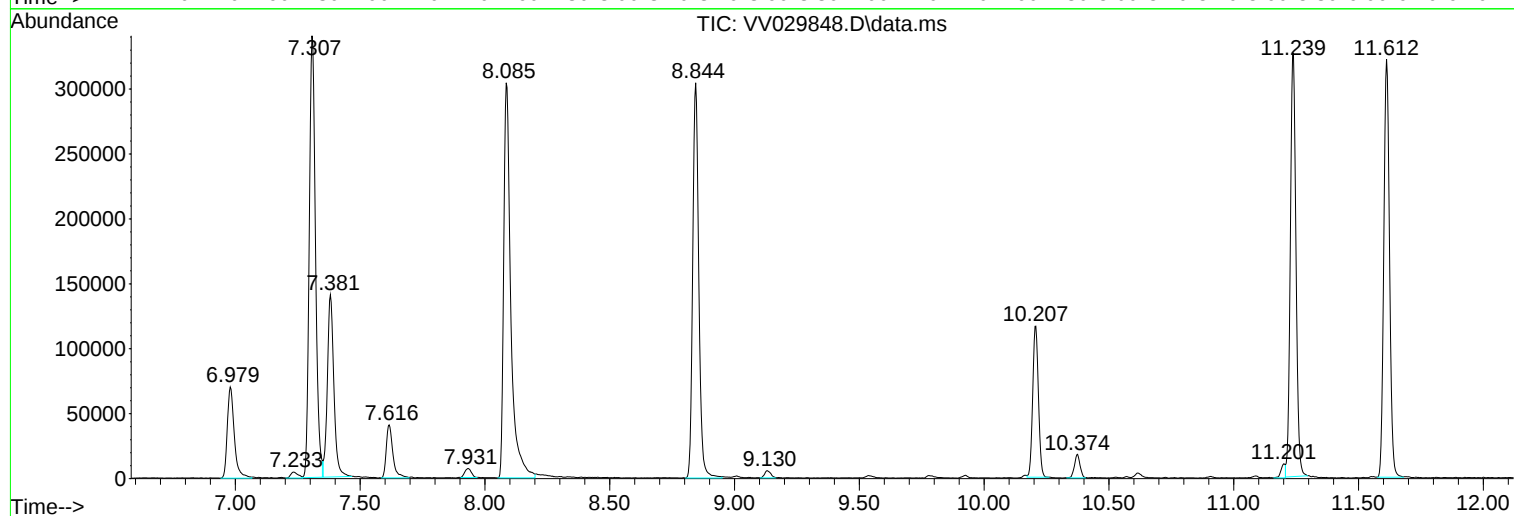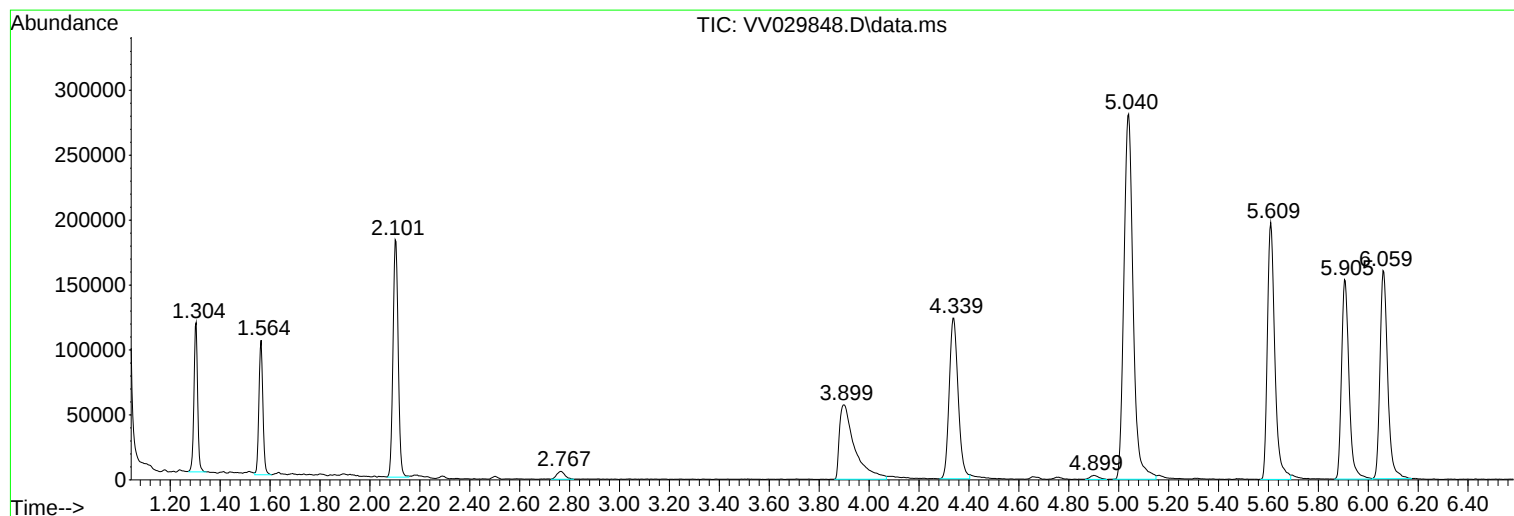

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029848.D
Acq On : 14 Jan 2023 10:55
Operator : SY/MD
Sample : 01149-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029848.D
Acq On : 14 Jan 2023 10:55
Operator : SY/MD
Sample : 01149-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc