

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029849.D
 Acq On : 14 Jan 2023 11:16
 Operator : SY/MD
 Sample : 01149-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL57

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029849.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	94	rVB	114942	122273	16.72%	1.881%
2	1.564	156	163	177	rVB	101434	113650	15.54%	1.748%
3	2.108	321	332	346	rBV	183516	266662	36.47%	4.101%
4	2.767	521	537	560	rVB	32522	68729	9.40%	1.057%
5	3.899	878	889	928	rBV	68694	245685	33.60%	3.779%
6	4.342	1011	1027	1055	rBV	123884	310616	42.48%	4.777%
7	4.912	1191	1204	1216	rVB5	3936	9569	1.31%	0.147%
8	5.043	1228	1245	1282	rBV2	284509	731267	100.00%	11.247%
9	5.612	1408	1422	1450	rBV	213919	446613	61.07%	6.869%
10	5.911	1503	1515	1538	rBV	92601	186732	25.54%	2.872%
11	6.066	1549	1563	1596	rBV	162850	346211	47.34%	5.325%
12	6.982	1836	1848	1871	rBV2	71012	135129	18.48%	2.078%
13	7.310	1937	1950	1964	rBV	340454	604359	82.65%	9.295%
14	7.384	1964	1973	1992	rVB	103100	191288	26.16%	2.942%
15	7.616	2034	2045	2063	rBV	41447	75444	10.32%	1.160%
16	7.931	2131	2143	2161	rBV	8111	16454	2.25%	0.253%
17	8.088	2180	2192	2225	rBV	324792	628846	85.99%	9.672%
18	8.844	2416	2427	2460	rBV	327578	555221	75.93%	8.539%
19	9.779	2709	2718	2732	rBV5	5353	11099	1.52%	0.171%
20	10.207	2830	2851	2871	rBV	129847	208394	28.50%	3.205%
21	10.374	2892	2903	2917	rBV	22903	38147	5.22%	0.587%
22	10.612	2969	2977	2992	rVB4	4392	9301	1.27%	0.143%
23	11.201	3152	3160	3162	rBV	13694	15809	2.16%	0.243%
24	11.239	3162	3172	3193	rVB	377911	584854	79.98%	8.995%
25	11.612	3275	3288	3311	rBV	352445	557019	76.17%	8.567%
26	12.242	3470	3484	3495	rVB	6505	10811	1.48%	0.166%
27	14.030	4027	4040	4049	rBV2	7185	11749	1.61%	0.181%




Sum of corrected areas: 6501931

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029849.D
Acq On : 14 Jan 2023 11:16
Operator : SY/MD
Sample : 01149-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

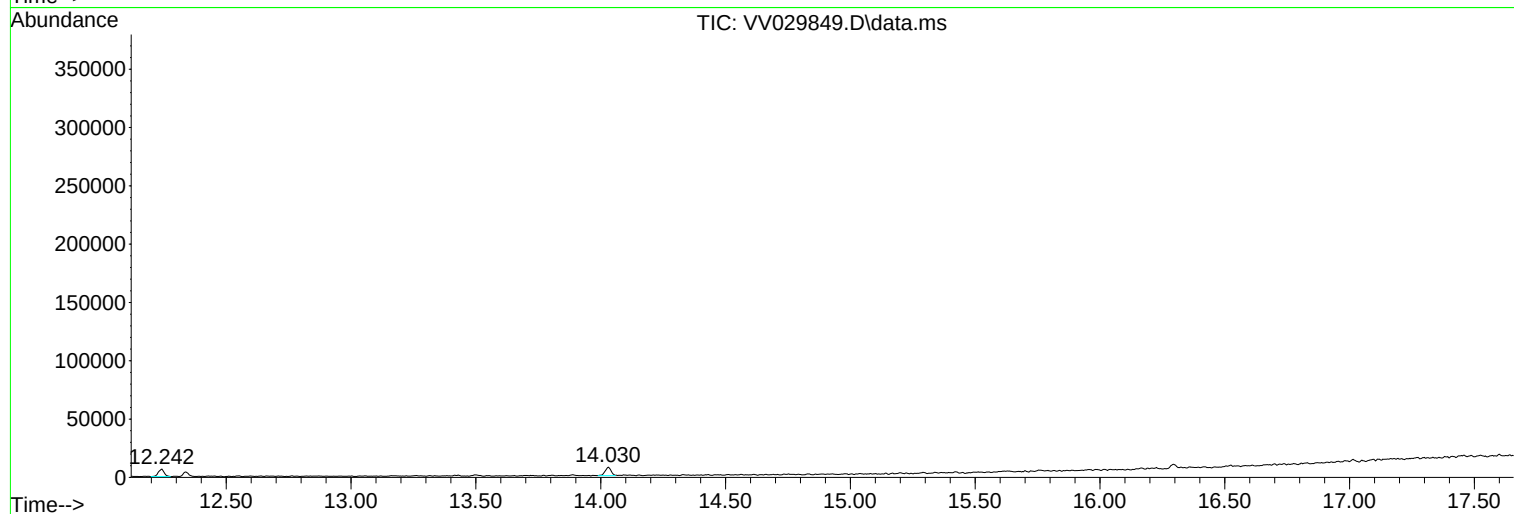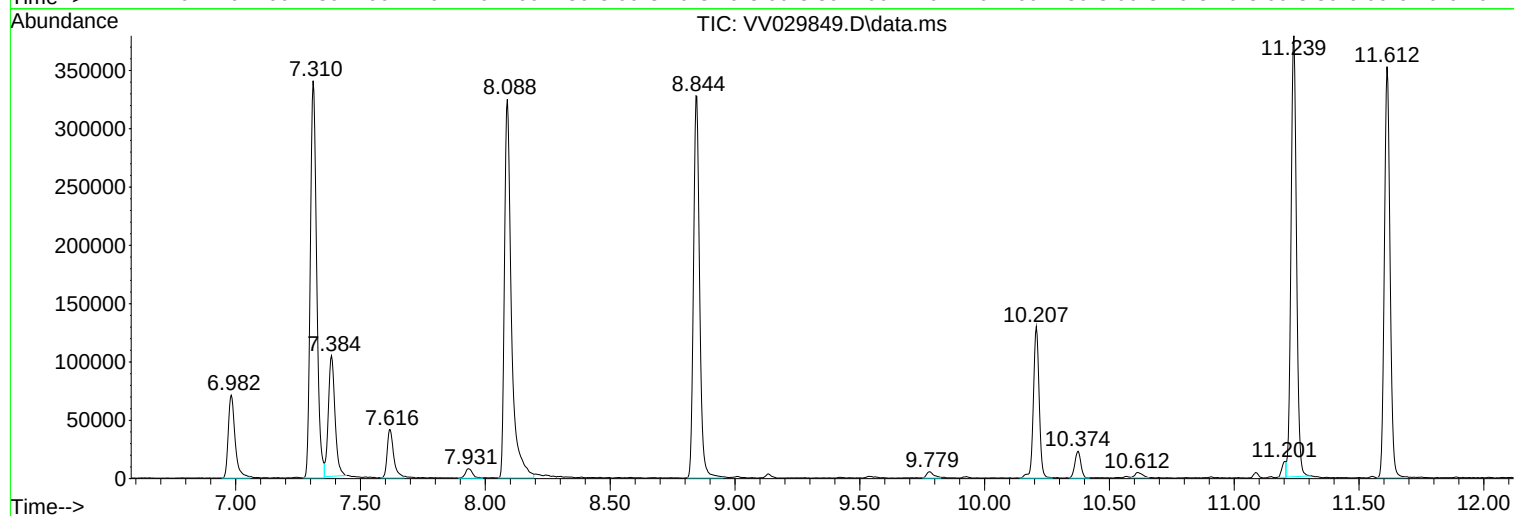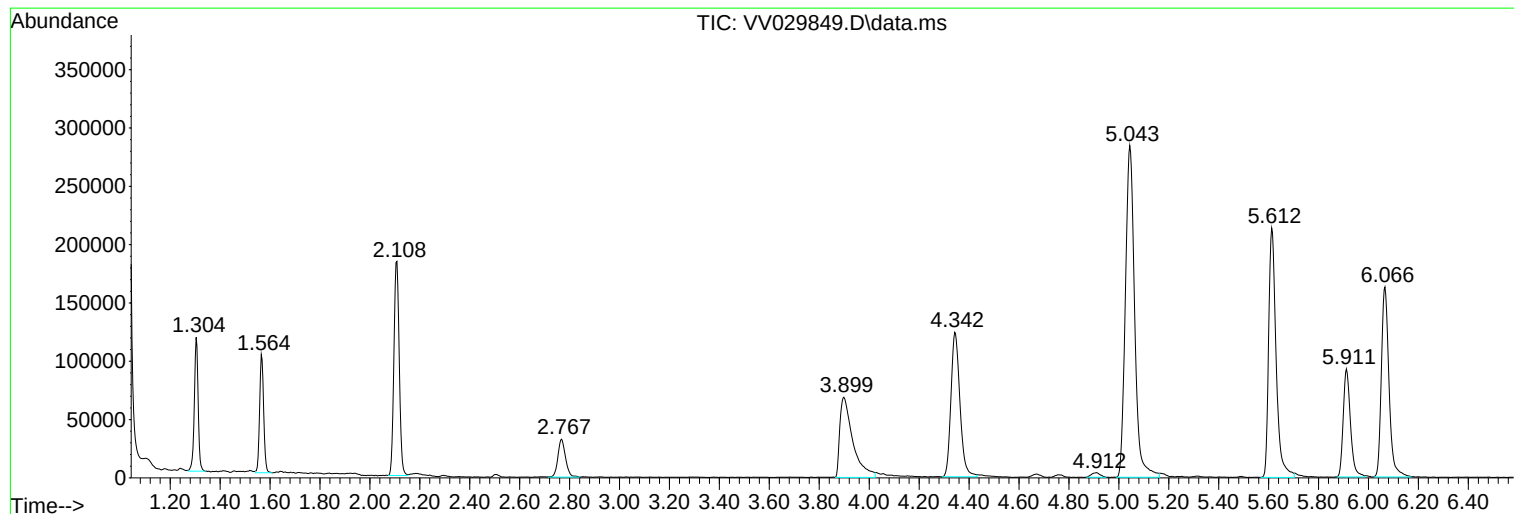

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029849.D
Acq On : 14 Jan 2023 11:16
Operator : SY/MD
Sample : 01149-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029849.D
Acq On : 14 Jan 2023 11:16
Operator : SY/MD
Sample : 01149-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
