

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029853.D
 Acq On : 14 Jan 2023 12:53
 Operator : SY/MD
 Sample : 01149-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0L56

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	96	rVB	112059	114719	7.25%	1.433%
2	1.564	155	163	178	rVB	101149	113839	7.20%	1.422%
3	2.105	321	331	346	rBV	183326	262331	16.58%	3.278%
4	2.764	517	536	555	rBV2	29826	66225	4.19%	0.827%
5	3.899	876	889	921	rBV2	70385	260151	16.44%	3.250%
6	4.339	1008	1026	1061	rBV	127484	327990	20.73%	4.098%
7	5.040	1227	1244	1277	rBV2	291814	743639	47.00%	9.291%
8	5.609	1408	1421	1462	rBV	227759	477762	30.20%	5.969%
9	5.905	1499	1513	1549	rBV	789824	1582082	100.00%	19.767%
10	6.063	1549	1562	1601	rVB	172116	370988	23.45%	4.635%
11	6.979	1836	1847	1876	rBV	73215	138540	8.76%	1.731%
12	7.307	1937	1949	1963	rBV	351906	625674	39.55%	7.817%
13	7.381	1963	1972	1993	rVB	126340	229929	14.53%	2.873%
14	7.616	2034	2045	2061	rBV2	43639	77415	4.89%	0.967%
15	8.085	2180	2191	2244	rBV	322346	647874	40.95%	8.095%
16	8.844	2415	2427	2457	rBV	351278	591048	37.36%	7.385%
17	10.204	2840	2850	2872	rVB	130641	208021	13.15%	2.599%
18	11.239	3161	3172	3193	rVB	383104	604873	38.23%	7.558%
19	11.612	3277	3288	3307	rBV	358873	560445	35.42%	7.002%




Sum of corrected areas: 8003545

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029853.D
Acq On : 14 Jan 2023 12:53
Operator : SY/MD
Sample : 01149-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

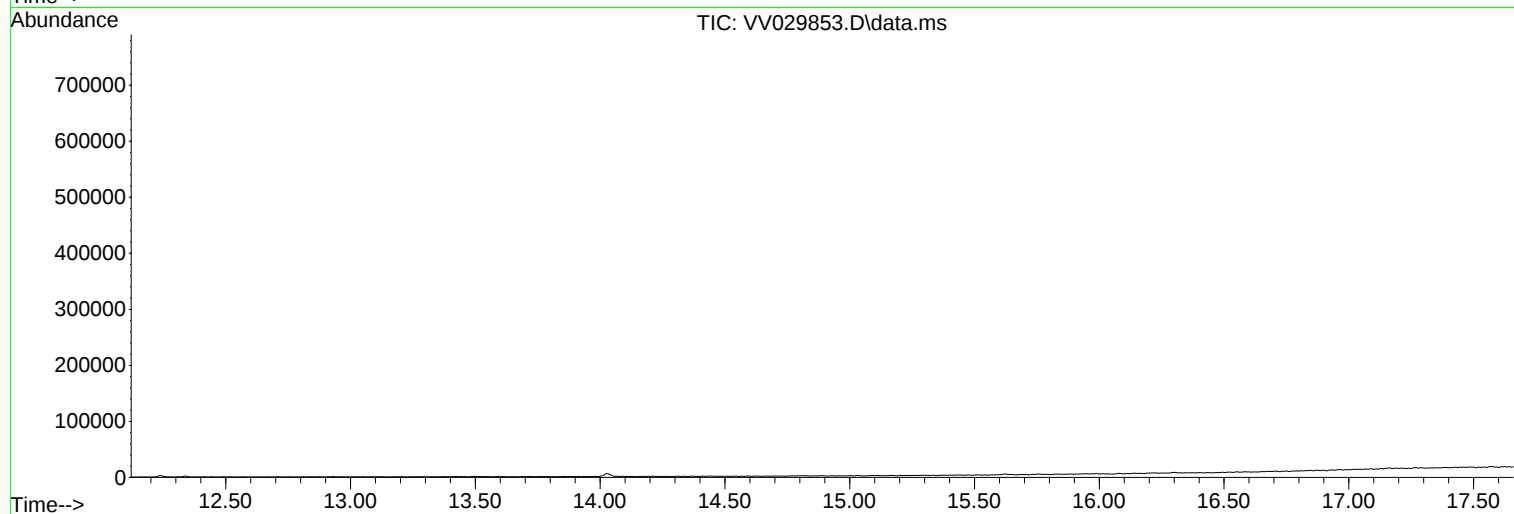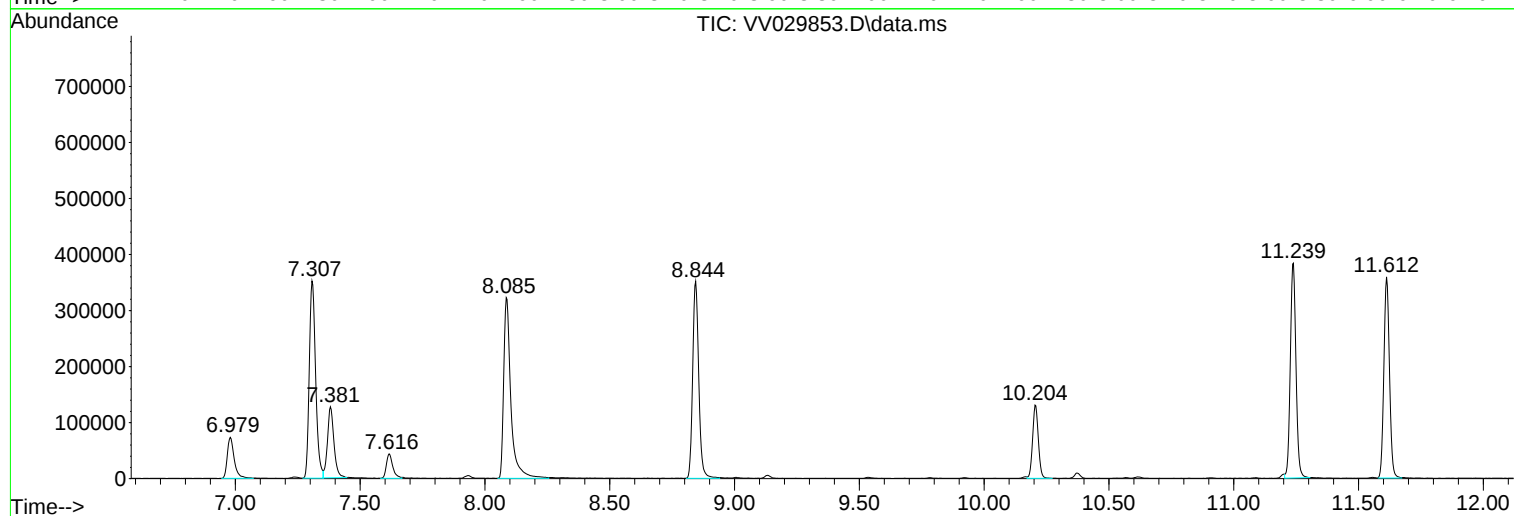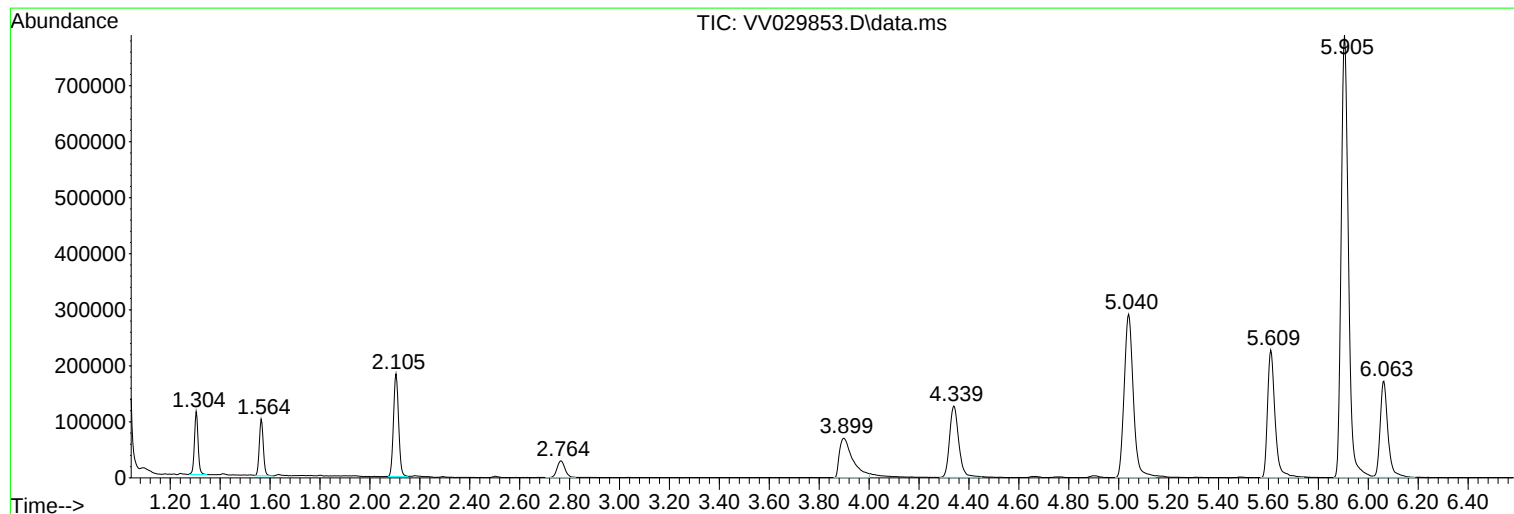

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029853.D
Acq On : 14 Jan 2023 12:53
Operator : SY/MD
Sample : 01149-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029853.D
Acq On : 14 Jan 2023 12:53
Operator : SY/MD
Sample : 01149-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc