

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029854.D
 Acq On : 14 Jan 2023 13:17
 Operator : SY/MD
 Sample : 01149-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0L54

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	93	rVB	118646	119280	3.89%	1.233%
2	1.565	156	163	177	rVB	100147	111555	3.63%	1.153%
3	2.105	320	331	344	rBV	191400	278620	9.08%	2.879%
4	2.761	522	535	558	rVB3	29099	61906	2.02%	0.640%
5	3.899	876	889	920	rBV3	100888	337692	11.00%	3.490%
6	4.339	1008	1026	1054	rBV2	129826	328237	10.69%	3.392%
7	5.040	1226	1244	1278	rBV2	293398	750533	24.45%	7.756%
8	5.609	1407	1421	1453	rBV	210504	443108	14.44%	4.579%
9	5.905	1498	1513	1549	rBV	1544407	3069510	100.00%	31.718%
10	6.063	1549	1562	1599	rVB	174231	376186	12.26%	3.887%
11	6.979	1835	1847	1872	rBV	74413	140117	4.56%	1.448%
12	7.307	1937	1949	1962	rBV	355237	627462	20.44%	6.484%
13	7.381	1962	1972	1999	rVB	213545	386658	12.60%	3.995%
14	7.616	2034	2045	2071	rBV	43256	79883	2.60%	0.825%
15	8.085	2180	2191	2232	rBV	330643	647885	21.11%	6.695%
16	8.844	2413	2427	2452	rBV	327691	549268	17.89%	5.676%
17	10.204	2840	2850	2869	rVB	131695	207028	6.74%	2.139%
18	10.371	2890	2902	2914	rVB2	22237	36318	1.18%	0.375%
19	11.236	3161	3171	3189	rVB	358812	561737	18.30%	5.805%
20	11.612	3277	3288	3313	rVB	358990	564385	18.39%	5.832%




Sum of corrected areas: 9677368

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029854.D
Acq On : 14 Jan 2023 13:17
Operator : SY/MD
Sample : 01149-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

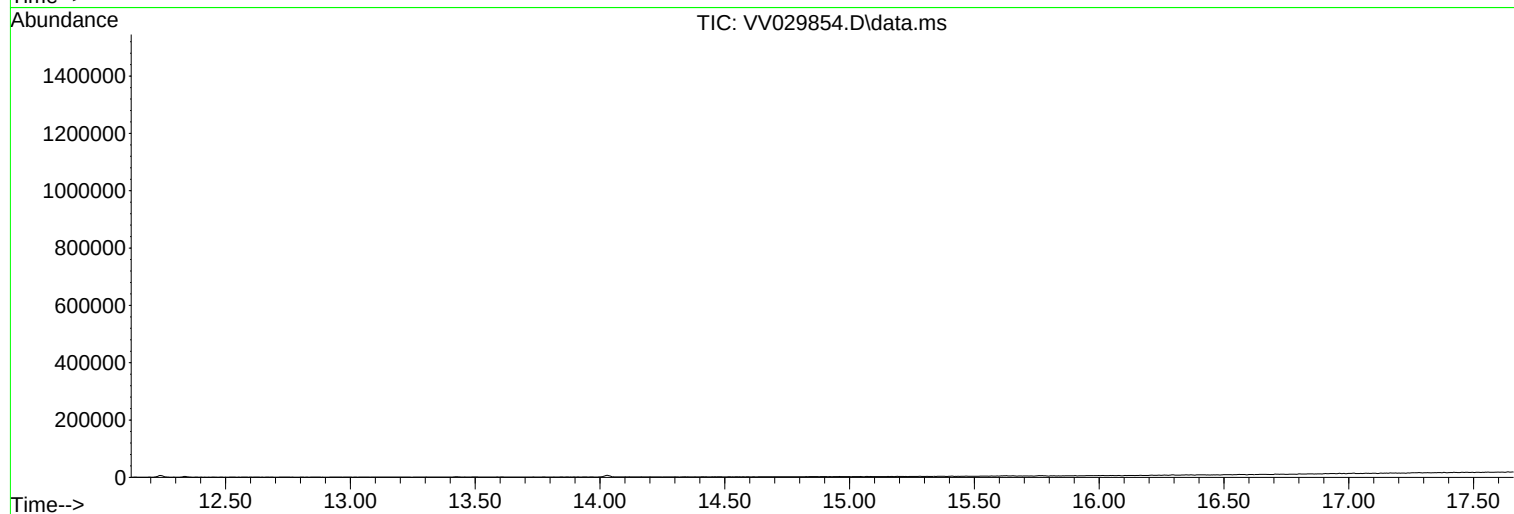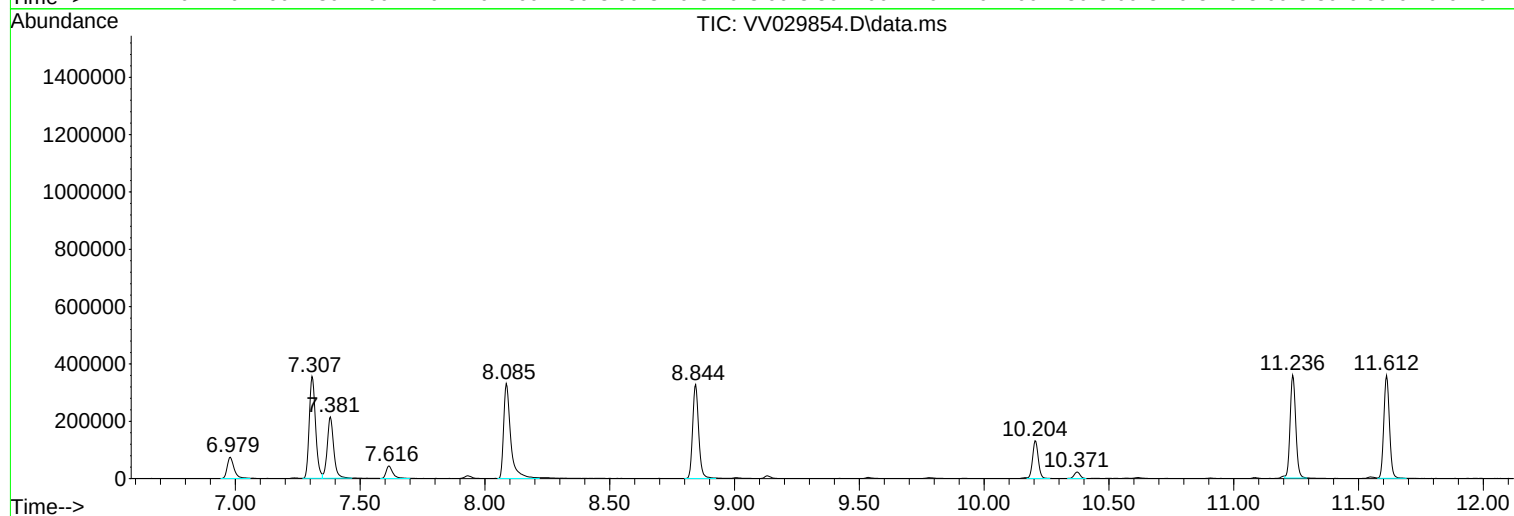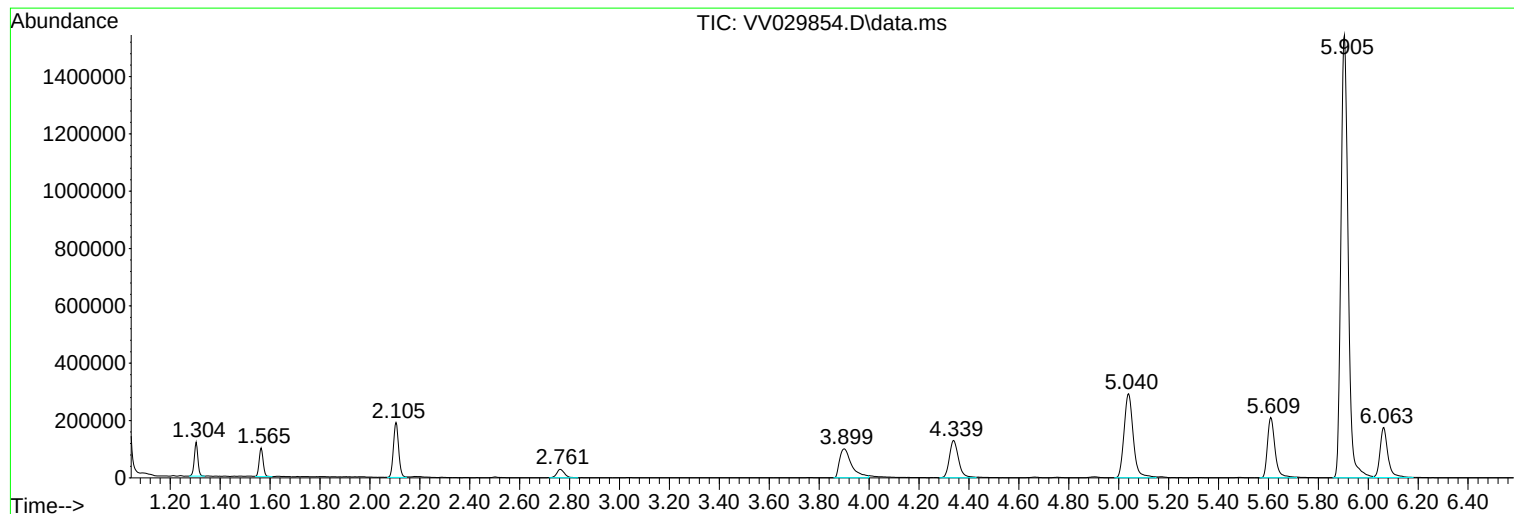

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029854.D
Acq On : 14 Jan 2023 13:17
Operator : SY/MD
Sample : 01149-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029854.D
Acq On : 14 Jan 2023 13:17
Operator : SY/MD
Sample : 01149-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0L54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
