

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029855.D
 Acq On : 14 Jan 2023 13:41
 Operator : SY/MD
 Sample : 01149-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	111130	111486	15.61%	1.983%
2	1.564	155	163	175	rVB	101488	113185	15.85%	2.013%
3	2.105	320	331	345	rBV	179376	258228	36.17%	4.592%
4	3.896	878	888	935	rBV	60269	244792	34.28%	4.353%
5	4.339	1009	1026	1049	rBV	126380	314650	44.07%	5.596%
6	5.040	1226	1244	1283	rBV2	275837	713995	100.00%	12.698%
7	5.609	1408	1421	1460	rBV	186655	395130	55.34%	7.027%
8	5.908	1503	1514	1532	rBV7	4092	8664	1.21%	0.154%
9	6.063	1546	1562	1596	rBV	158983	341297	47.80%	6.070%
10	6.979	1836	1847	1877	rBV	69017	134125	18.79%	2.385%
11	7.307	1937	1949	1988	rBV	331431	597878	83.74%	10.633%
12	7.616	2032	2045	2064	rBV	41271	76072	10.65%	1.353%
13	7.931	2133	2143	2153	rBV2	8970	15928	2.23%	0.283%
14	8.085	2179	2191	2236	rBV	314668	629299	88.14%	11.192%
15	8.844	2415	2427	2451	rBV	289738	483092	67.66%	8.591%
16	10.207	2840	2851	2866	rVB	125473	197828	27.71%	3.518%
17	10.371	2891	2902	2912	rBV	17848	28083	3.93%	0.499%
18	11.236	3156	3171	3192	rBV	283180	452151	63.33%	8.041%
19	11.612	3276	3288	3312	rVB	306358	483640	67.74%	8.601%
20	12.236	3474	3482	3494	rBV2	6292	10121	1.42%	0.180%
21	14.027	4030	4039	4050	rVB	8090	13276	1.86%	0.236%




Sum of corrected areas: 5622920

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029855.D
Acq On : 14 Jan 2023 13:41
Operator : SY/MD
Sample : 01149-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

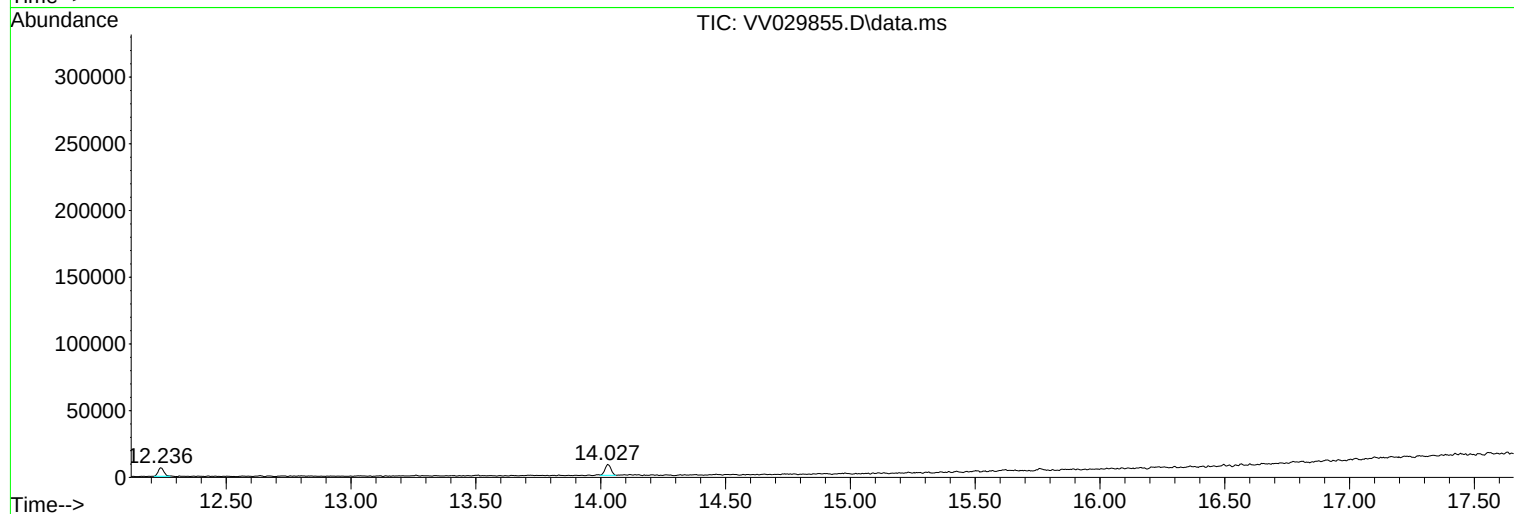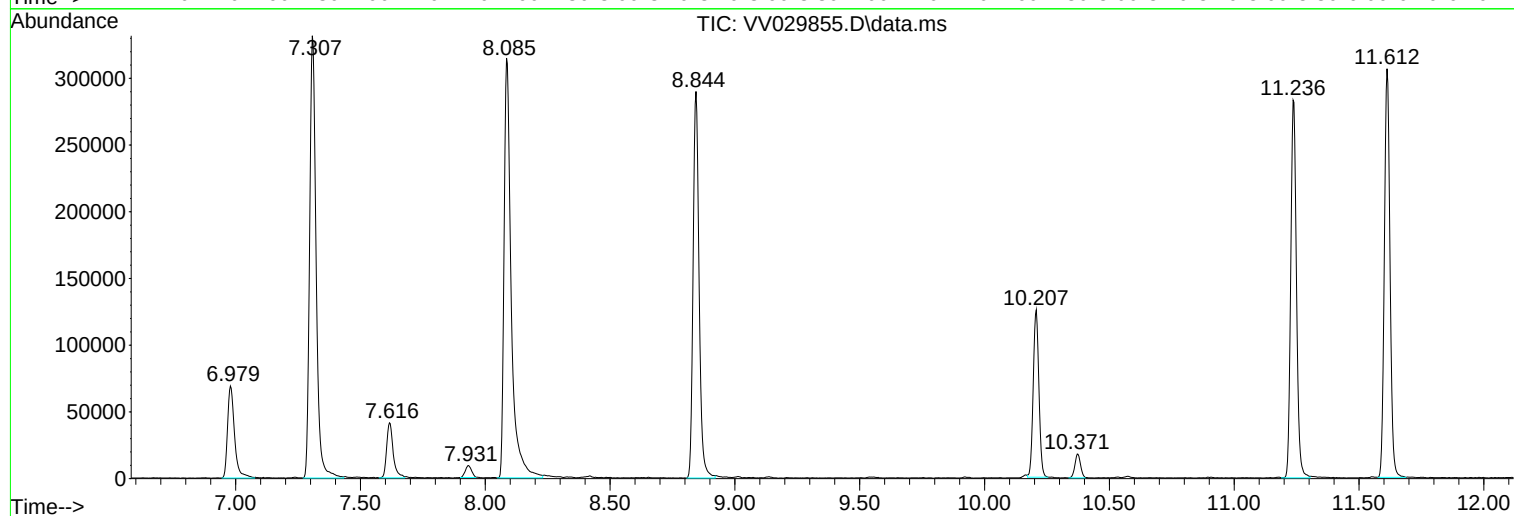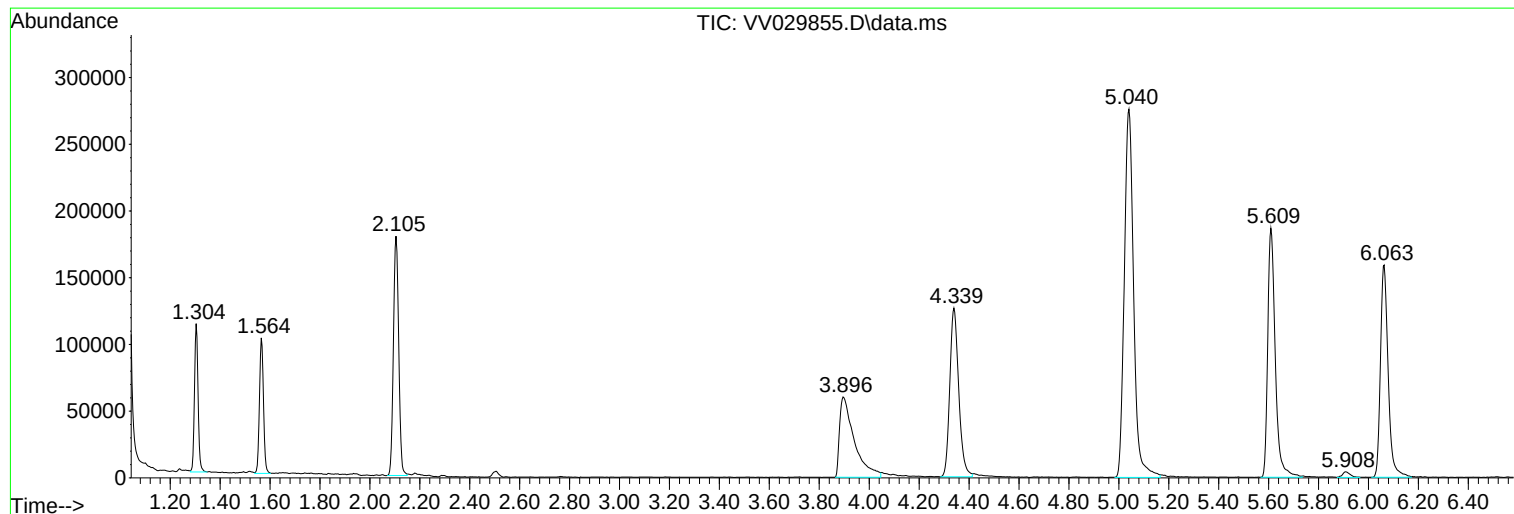

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029855.D
Acq On : 14 Jan 2023 13:41
Operator : SY/MD
Sample : 01149-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029855.D
Acq On : 14 Jan 2023 13:41
Operator : SY/MD
Sample : 01149-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
