

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029858.D
 Acq On : 14 Jan 2023 15:12
 Operator : SY/MD
 Sample : 01138-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1W7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	124680	125511	16.00%	1.902%
2	1.564	156	163	179	rBV	109035	130569	16.64%	1.979%
3	1.802	233	237	250	rVB	13023	15449	1.97%	0.234%
4	2.105	322	331	348	rVB2	214024	339192	43.23%	5.141%
5	2.767	523	537	553	rBV2	7574	16591	2.11%	0.251%
6	3.185	652	667	684	rBV2	17288	36946	4.71%	0.560%
7	3.892	876	887	921	rBV	78202	266672	33.99%	4.042%
8	4.339	1009	1026	1063	rBV	135078	346255	44.13%	5.249%
9	4.596	1094	1106	1124	rVB3	4660	11508	1.47%	0.174%
10	5.040	1227	1244	1285	rBV2	305686	784592	100.00%	11.893%
11	5.609	1408	1421	1453	rBV	201449	422945	53.91%	6.411%
12	5.908	1502	1514	1536	rBV2	87122	176812	22.54%	2.680%
13	6.063	1548	1562	1591	rBV	177139	373891	47.65%	5.667%
14	6.979	1833	1847	1877	rBV	74010	143577	18.30%	2.176%
15	7.307	1937	1949	1968	rBV	385651	695859	88.69%	10.548%
16	7.616	2031	2045	2071	rBV	45884	84973	10.83%	1.288%
17	7.934	2135	2144	2149	rBV3	4455	8063	1.03%	0.122%
18	7.966	2149	2154	2168	rVB3	9375	16102	2.05%	0.244%
19	8.085	2180	2191	2231	rBV	358517	689912	87.93%	10.458%
20	8.844	2415	2427	2453	rBV	327333	545478	69.52%	8.268%
21	9.136	2507	2518	2527	rBV2	6140	10841	1.38%	0.164%
22	10.204	2841	2850	2867	rVB	134265	212636	27.10%	3.223%
23	10.374	2889	2903	2912	rBV	11052	17826	2.27%	0.270%
24	11.236	3161	3171	3194	rVB	337758	523010	66.66%	7.928%
25	11.612	3275	3288	3310	rBV	375484	592281	75.49%	8.978%
26	14.030	4027	4040	4050	rBV	5340	9700	1.24%	0.147%




Sum of corrected areas: 6597191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029858.D
Acq On : 14 Jan 2023 15:12
Operator : SY/MD
Sample : 01138-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

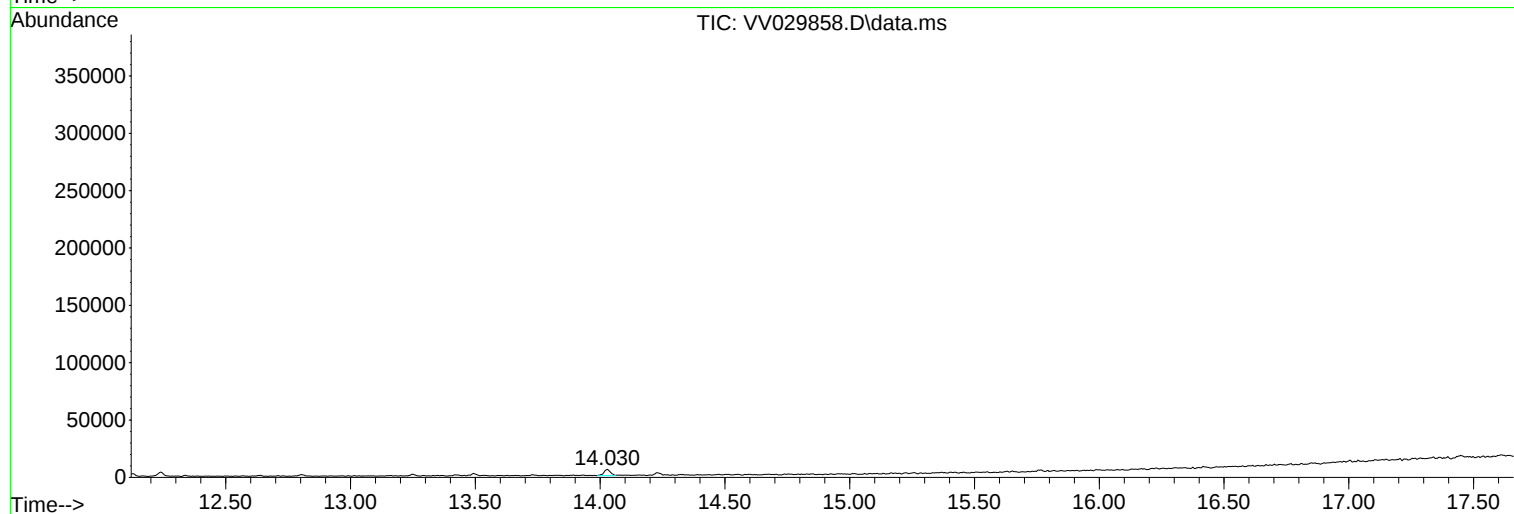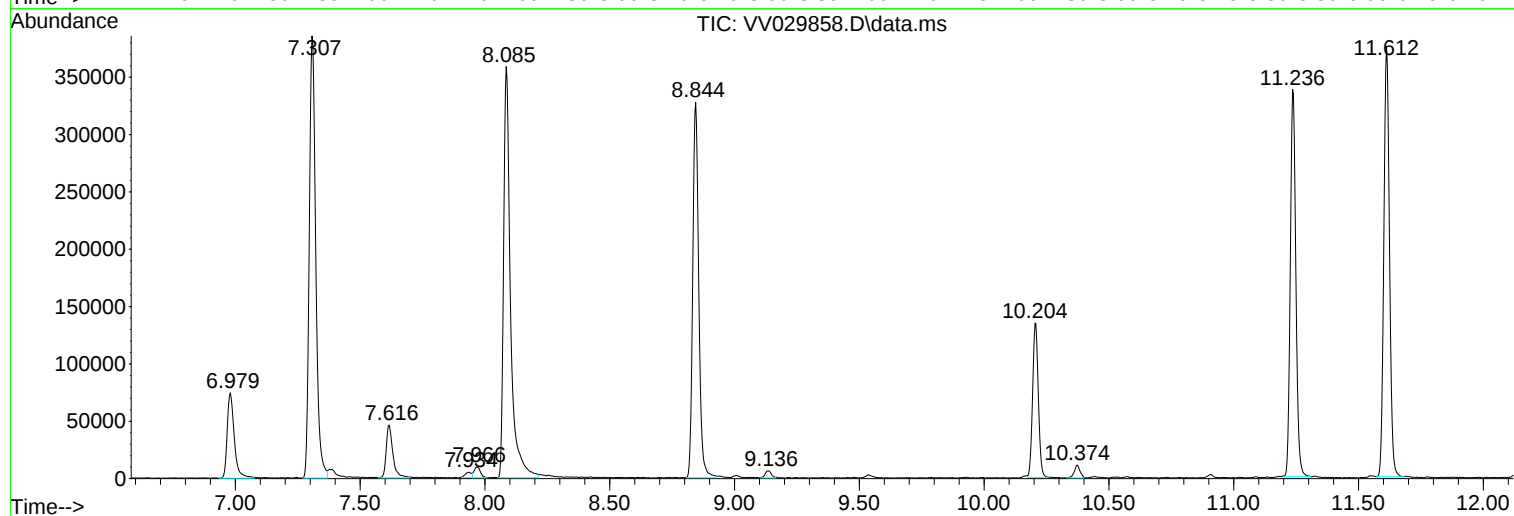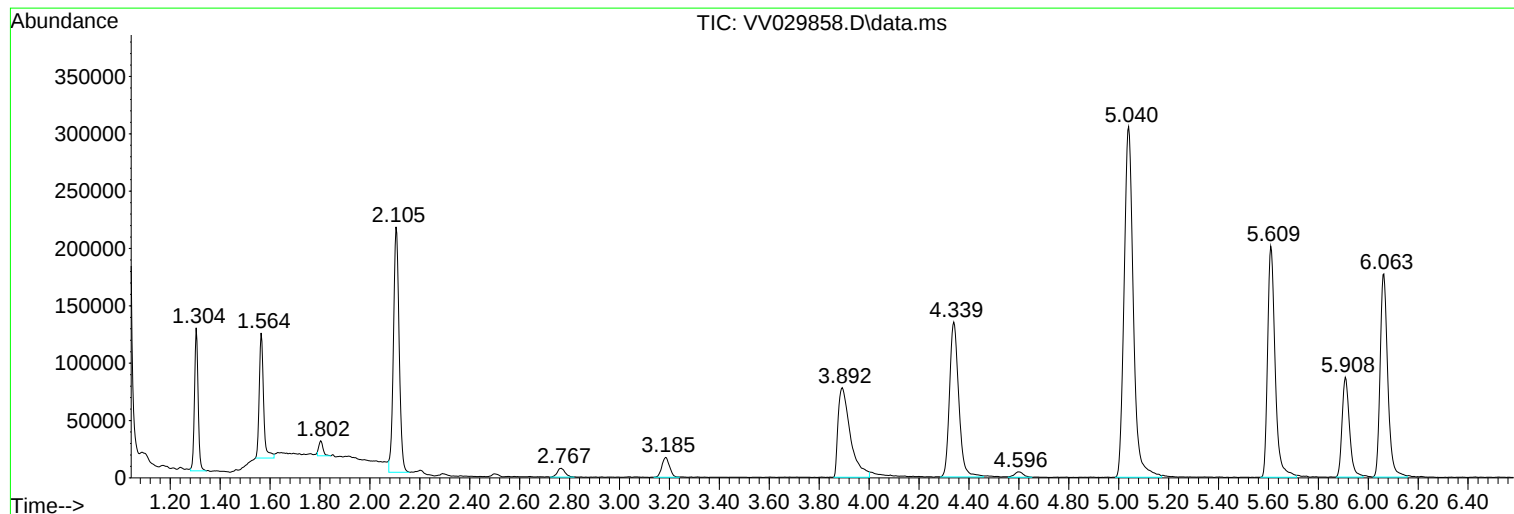

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029858.D
Acq On : 14 Jan 2023 15:12
Operator : SY/MD
Sample : 01138-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029858.D
Acq On : 14 Jan 2023 15:12
Operator : SY/MD
Sample : 01138-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------