

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
 Data File : VV029860.D
 Acq On : 14 Jan 2023 16:00
 Operator : SY/MD
 Sample : 01138-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH1X1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rVB	114221	113390	15.16%	1.569%
2	1.564	155	163	176	rVB	102118	115042	15.38%	1.592%
3	2.105	320	331	348	rVB2	202808	313099	41.85%	4.332%
4	2.764	520	536	556	rBV	267122	561262	75.02%	7.765%
5	3.185	655	667	679	rBV	6960	13677	1.83%	0.189%
6	3.892	876	887	930	rBV	69208	250058	33.42%	3.459%
7	4.339	1009	1026	1053	rBV2	130020	332017	44.38%	4.593%
8	4.596	1094	1106	1126	rVB3	6090	13903	1.86%	0.192%
9	5.040	1227	1244	1289	rBV2	292432	748172	100.00%	10.351%
10	5.609	1408	1421	1448	rBV	205665	424456	56.73%	5.872%
11	5.905	1500	1513	1546	rBV	274318	551918	73.77%	7.635%
12	6.063	1549	1562	1590	rVV	169684	350954	46.91%	4.855%
13	6.979	1835	1847	1874	rBV	71732	137735	18.41%	1.905%
14	7.307	1936	1949	1965	rBV	348703	622353	83.18%	8.610%
15	7.384	1966	1973	1997	rVB2	26087	51330	6.86%	0.710%
16	7.616	2034	2045	2068	rBV	42691	75990	10.16%	1.051%
17	7.934	2130	2144	2149	rBV4	4122	8245	1.10%	0.114%
18	7.969	2149	2155	2166	rVB3	5215	9050	1.21%	0.125%
19	8.085	2179	2191	2228	rBV	332564	640436	85.60%	8.860%
20	8.844	2413	2427	2463	rBV	319103	535986	71.64%	7.415%
21	9.130	2509	2516	2527	rBV2	6271	10028	1.34%	0.139%
22	9.554	2635	2648	2661	rBV5	7770	16903	2.26%	0.234%
23	10.204	2840	2850	2867	rVB	128459	207029	27.67%	2.864%
24	10.371	2894	2902	2913	rVB2	11133	17684	2.36%	0.245%
25	11.236	3159	3171	3193	rBV	346814	548817	73.35%	7.593%
26	11.612	3276	3288	3310	rBV	357880	558829	74.69%	7.731%




Sum of corrected areas: 7228363

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029860.D
Acq On : 14 Jan 2023 16:00
Operator : SY/MD
Sample : 01138-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

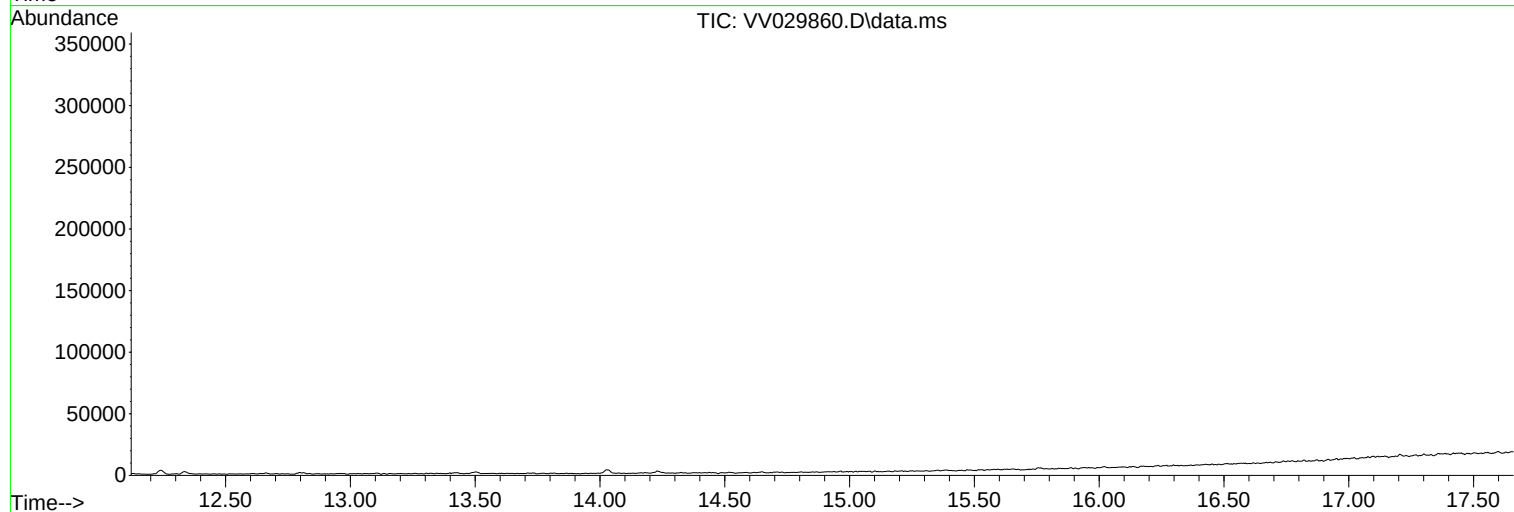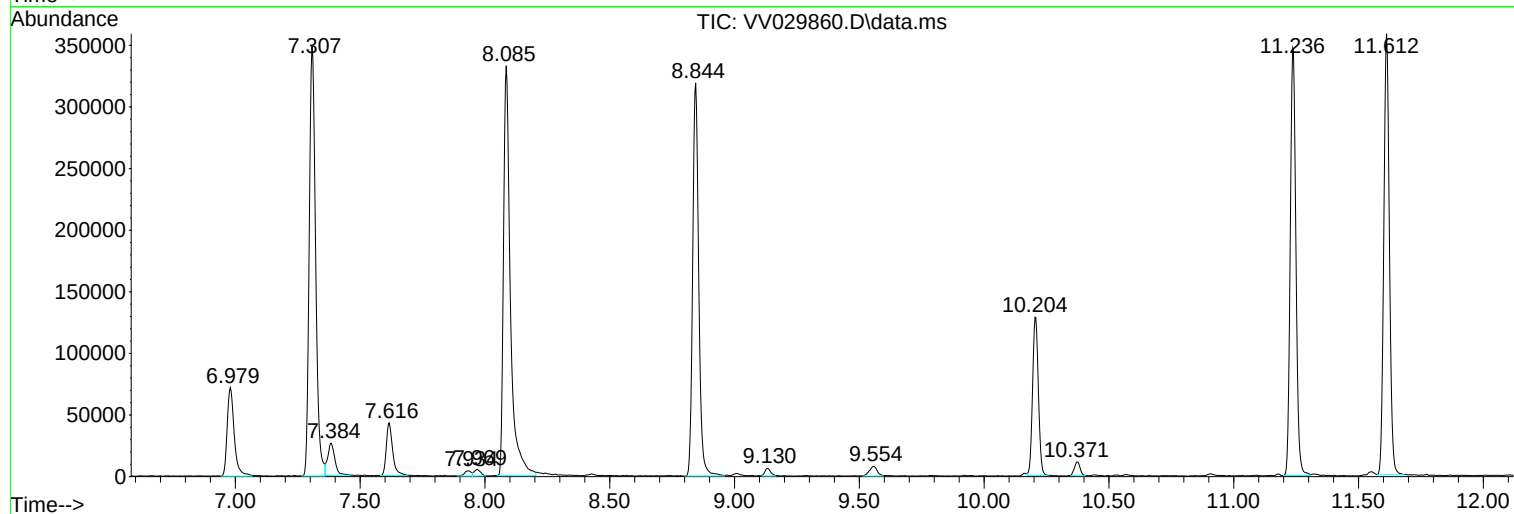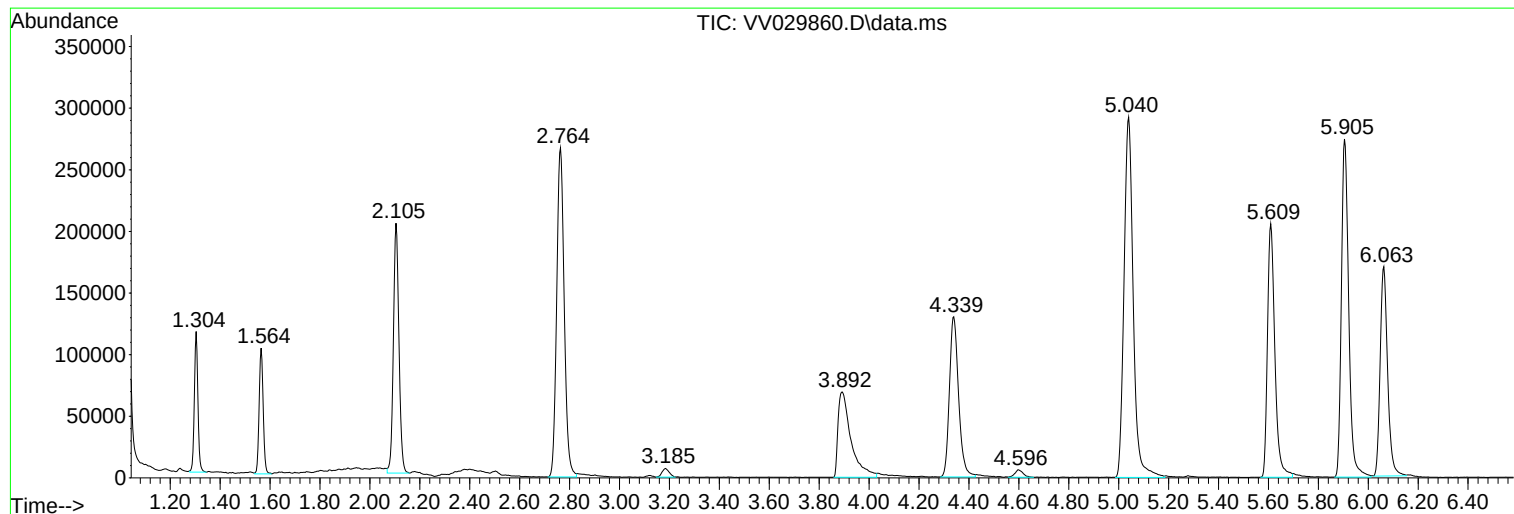

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029860.D
Acq On : 14 Jan 2023 16:00
Operator : SY/MD
Sample : 01138-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029860.D
Acq On : 14 Jan 2023 16:00
Operator : SY/MD
Sample : 01138-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH1X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------