


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011323\
Data File : VV029795.D
Acq On : 13 Jan 2023 09:11
Operator : SY/MD
Sample : BFB212
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB212

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 12 22:05:54 2023

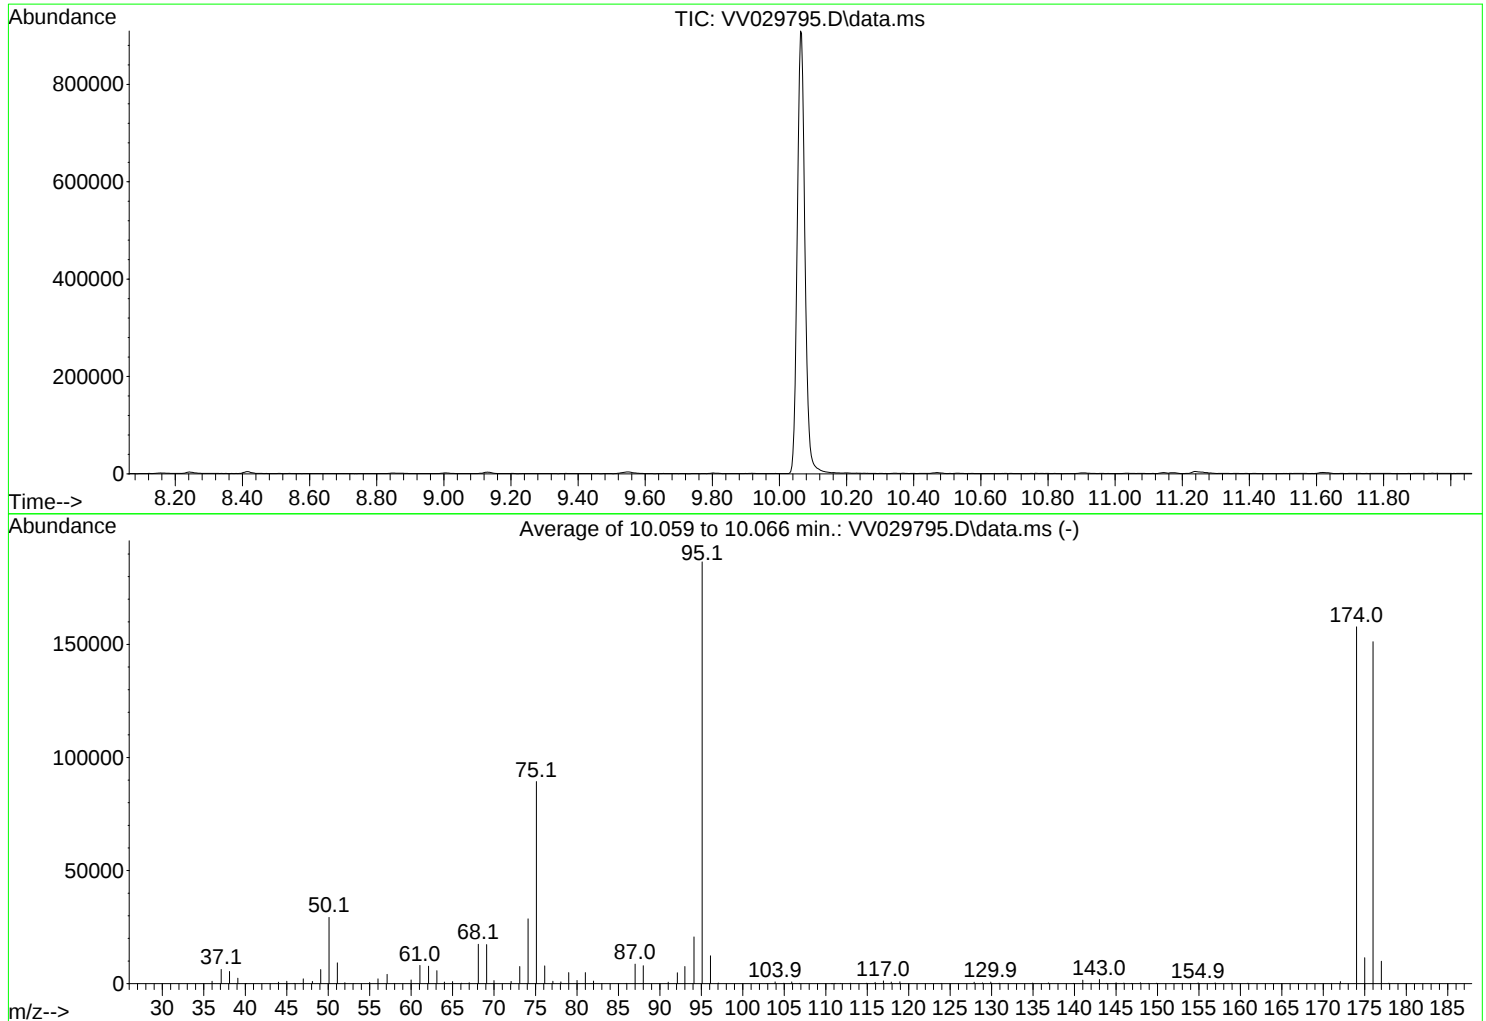

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	29317	PASS
75	95	30	80	47.9	89352	PASS
95	95	100	100	100.0	186517	PASS
96	95	5	9	6.6	12284	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.6	157781	PASS
175	174	5	9	7.3	11495	PASS
176	174	95	105	95.8	151189	PASS
177	176	5	10	6.6	9943	PASS

m/z	Abundance
40.00	166.0
44.00	486.0
207.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
36.00	1107.0
37.10	6033.0
38.10	5127.0
39.10	2250.0
40.00	184.0
43.00	107.0
44.10	1032.0
45.00	999.0
45.90	156.0
47.00	2107.0
48.10	906.0
49.10	5788.0
50.10	28216.0
51.10	8877.0
52.00	451.0
53.10	116.0
55.00	462.0
56.00	1959.0
57.10	3923.0
58.00	145.0
60.00	1501.0
61.10	7745.0
62.10	7326.0
63.10	5483.0
64.00	715.0
65.00	901.0
66.10	180.0
67.00	397.0
68.10	16287.0
69.10	16536.0
70.00	1323.0
72.10	960.0
73.10	7225.0
74.10	27536.0
75.10	85192.0
76.10	7519.0
77.10	985.0
78.00	734.0
79.00	4703.0
80.00	1371.0
81.00	4623.0
82.00	1063.0
85.90	158.0
87.00	8447.0
88.00	7618.0
91.00	612.0
92.10	4612.0
93.00	7166.0
94.10	19480.0
95.10	175488.0
96.10	11743.0
97.00	316.0
103.90	700.0
105.00	259.0
105.90	790.0
106.90	123.0
110.70	110.0
111.10	124.0
111.80	116.0
112.90	170.0
115.00	239.0
115.90	525.0
117.00	1047.0
117.90	729.0
118.90	777.0
123.90	129.0
127.90	580.0
128.90	366.0
129.90	722.0
130.90	196.0
135.00	278.0
136.90	308.0
139.90	136.0
141.00	1448.0
142.00	201.0
143.00	1646.0
143.80	147.0
145.00	392.0
146.00	239.0
146.90	112.0
147.90	470.0
148.90	135.0
149.90	238.0
153.00	140.0
153.90	113.0
154.90	339.0
157.00	328.0
159.00	170.0
160.90	198.0
170.90	122.0
172.10	880.0
174.00	146112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

175.00	11036.0
176.00	138112.0
177.00	9247.0
177.90	254.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
36.00	1085.0
37.10	6496.0
38.10	5603.0
39.10	2496.0
40.00	174.0
43.00	111.0
44.00	1106.0
45.00	1075.0
45.90	154.0
47.00	2190.0
48.10	1020.0
49.10	6485.0
50.10	30288.0
51.10	9547.0
52.00	455.0
53.00	111.0
55.00	515.0
56.00	2234.0
57.10	4207.0
58.00	193.0
60.00	1703.0
61.10	8365.0
62.10	7918.0
63.10	5929.0
64.00	723.0
65.00	982.0
66.10	193.0
67.00	417.0
68.10	18080.0
69.10	17952.0
70.00	1418.0
72.00	1014.0
73.10	7787.0
74.10	29448.0
75.10	92536.0
76.10	8205.0
77.10	1047.0
78.10	797.0
79.00	5058.0
80.00	1442.0
81.00	5024.0
82.00	1151.0
83.00	136.0
86.00	193.0
87.00	8979.0
88.00	8112.0
91.00	669.0
92.10	5042.0
93.00	7783.0
94.10	21280.0
95.10	192960.0
96.10	12647.0
97.00	253.0
102.90	109.0
103.90	794.0
104.90	251.0
105.90	819.0
106.80	188.0
111.10	120.0
111.80	119.0
113.00	211.0
115.00	234.0
115.90	543.0
116.90	1232.0
117.90	764.0
119.00	903.0
123.90	162.0
127.90	699.0
128.90	399.0
129.90	731.0
130.90	262.0
135.00	284.0
136.80	343.0
139.90	148.0
141.00	1630.0
142.00	211.0
143.00	1914.0
143.90	178.0
145.00	434.0
146.00	276.0
146.90	152.0
148.00	440.0
148.90	152.0
149.90	252.0
153.00	155.0
154.00	122.0
154.90	389.0
157.00	364.0
158.90	203.0
160.90	258.0
171.00	170.0
172.00	954.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

174.00	163136.0
175.00	11819.0
176.00	155584.0
177.00	10305.0
177.90	260.0
207.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

m/z	Abundance
36.00	1018.0
37.10	6441.0
38.10	5458.0
39.10	2532.0
40.00	167.0
43.10	105.0
44.00	1154.0
45.00	1061.0
45.90	137.0
47.00	2087.0
48.10	977.0
49.10	6466.0
50.10	29448.0
51.10	9205.0
52.00	401.0
55.00	446.0
56.00	2206.0
57.10	4167.0
57.90	211.0
60.00	1753.0
61.00	8032.0
62.10	7837.0
63.10	5886.0
64.00	653.0
65.00	921.0
66.10	182.0
67.00	384.0
68.10	17960.0
69.10	17416.0
70.00	1371.0
72.00	979.0
73.10	7643.0
74.10	29008.0
75.10	90328.0
76.10	7889.0
77.10	1070.0
78.10	797.0
79.00	4997.0
80.00	1385.0
81.00	5028.0
82.00	1102.0
83.00	148.0
87.00	8504.0
88.00	7969.0
91.00	651.0
92.10	4883.0
93.00	7729.0
94.10	21272.0
95.10	191104.0
96.10	12463.0
97.10	213.0
102.90	109.0
103.90	852.0
104.90	248.0
105.90	708.0
106.80	225.0
111.10	108.0
111.80	122.0
113.00	178.0
114.90	194.0
116.00	568.0
116.90	1266.0
117.90	690.0
119.00	946.0
123.90	152.0
127.90	715.0
128.90	371.0
129.90	685.0
130.90	299.0
134.90	271.0
136.80	351.0
139.90	140.0
141.00	1653.0
142.00	213.0
143.00	1963.0
143.90	148.0
145.00	385.0
145.90	274.0
146.90	167.0
148.00	397.0
148.90	152.0
149.90	260.0
153.00	147.0
154.00	119.0
154.90	427.0
156.90	394.0
158.90	212.0
160.90	259.0
171.00	160.0
172.00	970.0
174.00	164096.0
175.00	11631.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212

176.00	159872.0
177.00	10278.0
177.90	214.0
207.10	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB212