

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
 Data File : VV019996.D
 Acq On : 14 Jan 2021 12:48
 Operator : SY/MD
 Sample : M1147-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T8

Quant Time: Jan 15 01:07:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 13 13:06:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	377468	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.858	117	360317	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.257	152	184136	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.306	65	155109	48.72	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 97.44%			
7) Chloroethane-d5	1.569	69	131486	51.74	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 103.48%			
11) 1,1-Dichloroethene-d2	2.110	63	235462	37.55	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 75.10%			
21) 2-Butanone-d5	3.891	46	203027	98.30	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 98.30%			
24) Chloroform-d	4.354	84	269266	46.95	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 93.90%			
26) 1,2-Dichloroethane-d4	5.035	65	194621	49.92	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 99.84%			
32) Benzene-d6	5.055	84	506925	49.85	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 99.70%			
36) 1,2-Dichloropropane-d6	6.074	67	159795	50.33	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 100.66%			
41) Toluene-d8	7.318	98	449095	48.73	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 97.46%			
43) trans-1,3-Dichloroprop...	7.624	79	72887	44.24	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 88.48%			
47) 2-Hexanone-d5	8.093	63	109203	85.79	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 85.79%			
57) 1,1,2,2-Tetrachloroeth...	10.222	84	190409	44.36	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 88.72%			
64) 1,2-Dichlorobenzene-d4	11.630	152	178645	50.23	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 100.46%			
Target Compounds					Qvalue	
13) Acetone	2.187	43	6121	3.35	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV019996.D
Acq On : 14 Jan 2021 12:48
Operator : SY/MD
Sample : M1147-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T8


Quant Time: Jan 15 01:07:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 13 13:06:01 2021
Response via : Initial Calibration

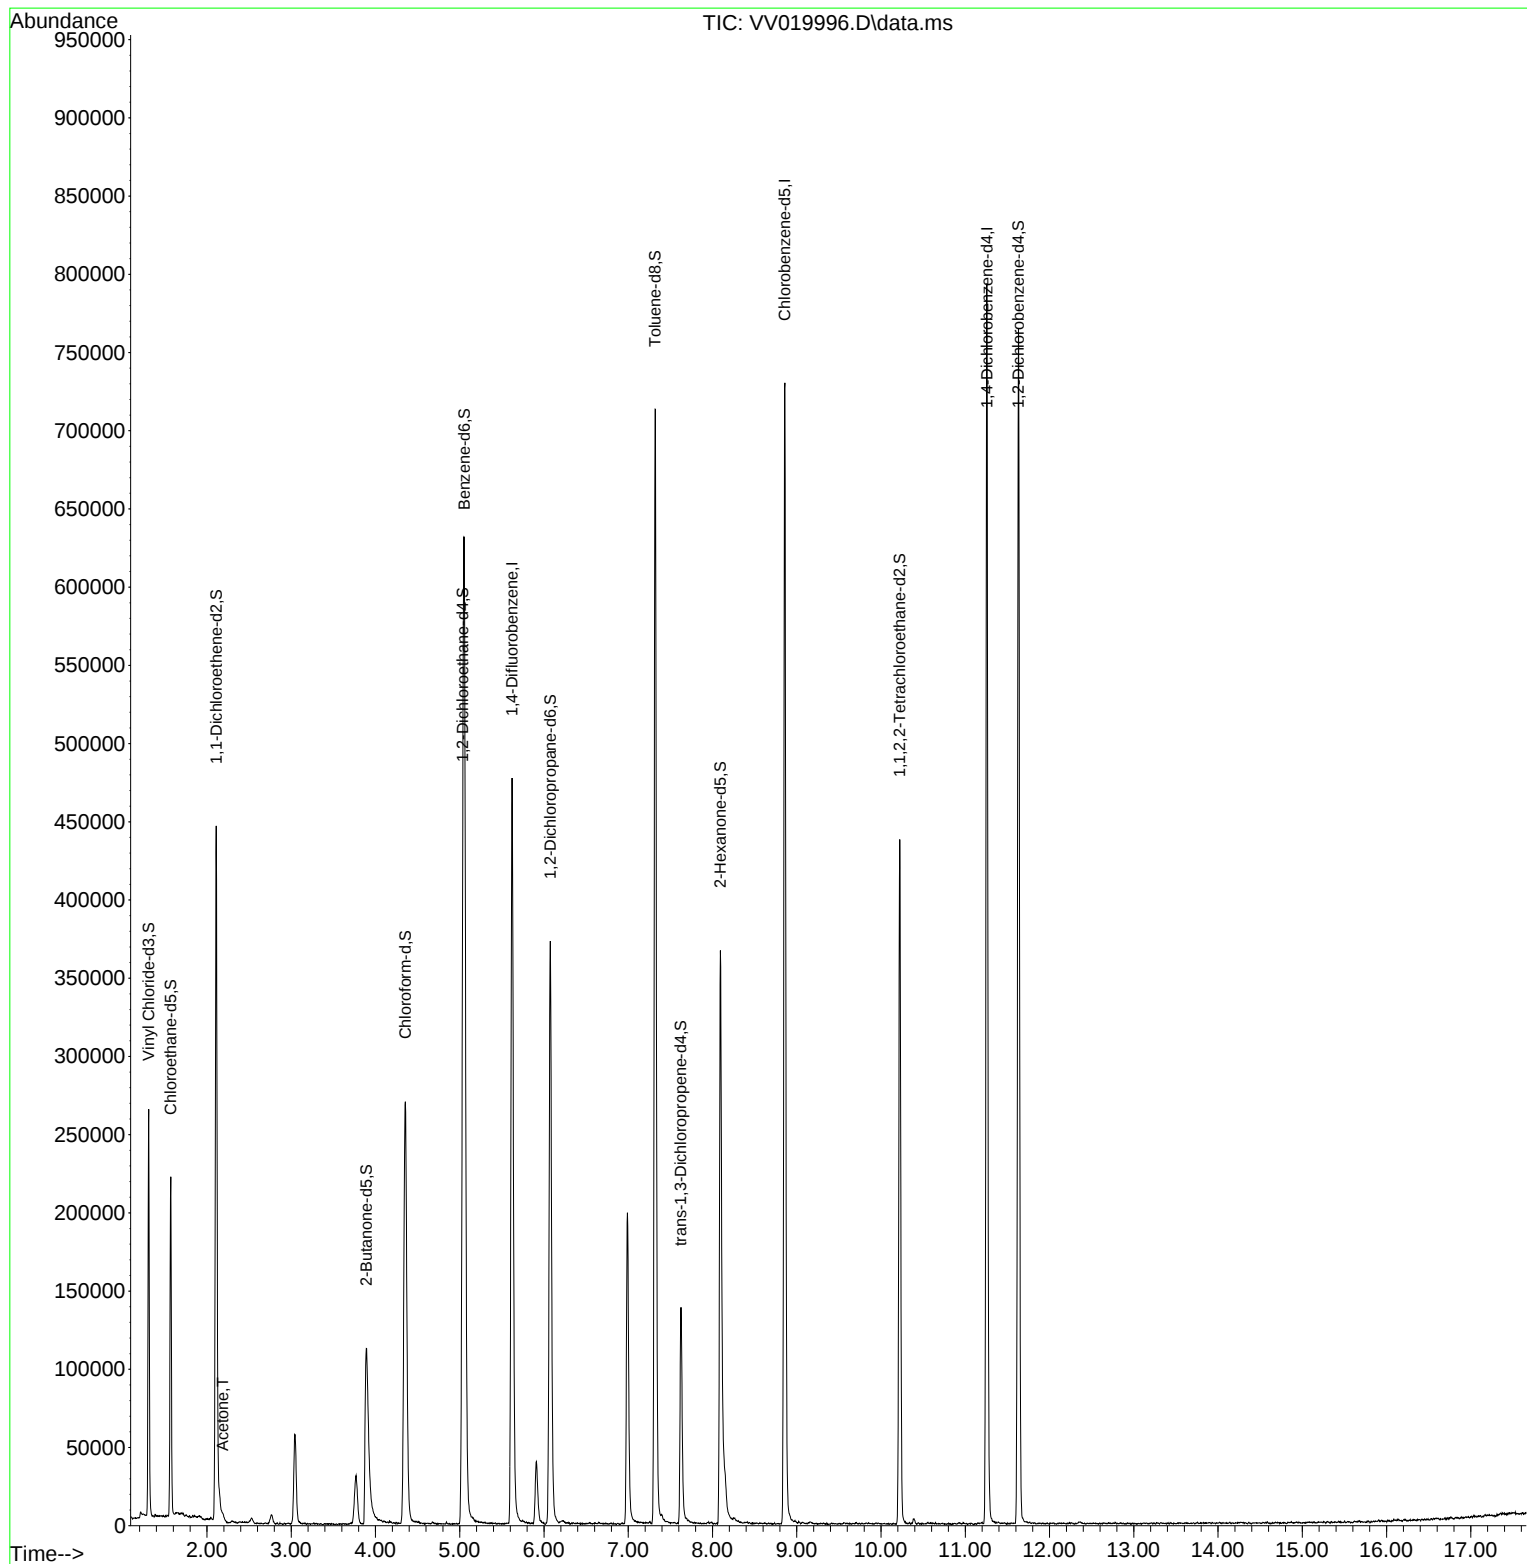

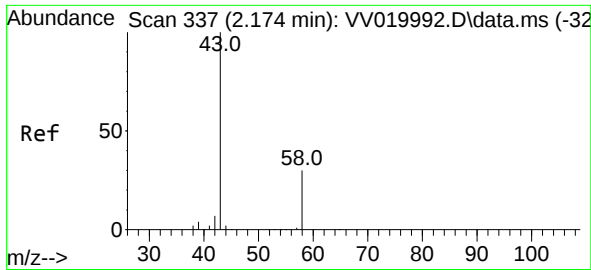

#13
 Acetone
 Concen: 3.35 ug/L
 RT: 2.187 min Scan# 341
 Delta R.T. 0.009 min
 Lab File: VV019996.D
 Acq: 14 Jan 2021 12:48

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4T8

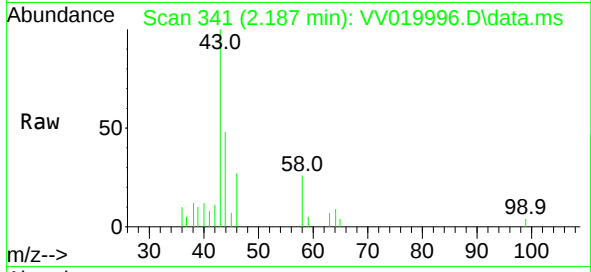

Tgt Ion: 43 Resp: 6121
 Ion Ratio Lower Upper
 43 100
 58 30.4 0.0 60.2

