

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
 Data File : VV019998.D
 Acq On : 14 Jan 2021 13:35
 Operator : SY/MD
 Sample : M1147-04 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y1

Quant Time: Jan 15 03:19:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 13 13:06:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	400668	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.859	117	382502	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.257	152	190618	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	154989	45.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.72%
7) Chloroethane-d5	1.569	69	131220	48.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.28%
11) 1,1-Dichloroethene-d2	2.110	63	238866	35.89	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.78%
21) 2-Butanone-d5	3.901	46	222711	101.58	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.58%
24) Chloroform-d	4.354	84	276863	45.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.96%
26) 1,2-Dichloroethane-d4	5.039	65	202382	48.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.80%
32) Benzene-d6	5.055	84	513093	47.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.06%
36) 1,2-Dichloropropane-d6	6.074	67	162569	48.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.46%
41) Toluene-d8	7.322	98	446826	45.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.34%
43) trans-1,3-Dichloroprop...	7.624	79	73660	42.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.22%
47) 2-Hexanone-d5	8.093	63	125730	93.04	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.04%
57) 1,1,2,2-Tetrachloroeth...	10.222	84	205916	45.19	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.38%
64) 1,2-Dichlorobenzene-d4	11.630	152	181809	49.38	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.76%
Target Compounds						
48) 2-Hexanone	8.151	43	11561	3.32	ug/L	Qvalue # 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV019998.D
Acq On : 14 Jan 2021 13:35
Operator : SY/MD
Sample : M1147-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y1


Quant Time: Jan 15 03:19:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 13 13:06:01 2021
Response via : Initial Calibration

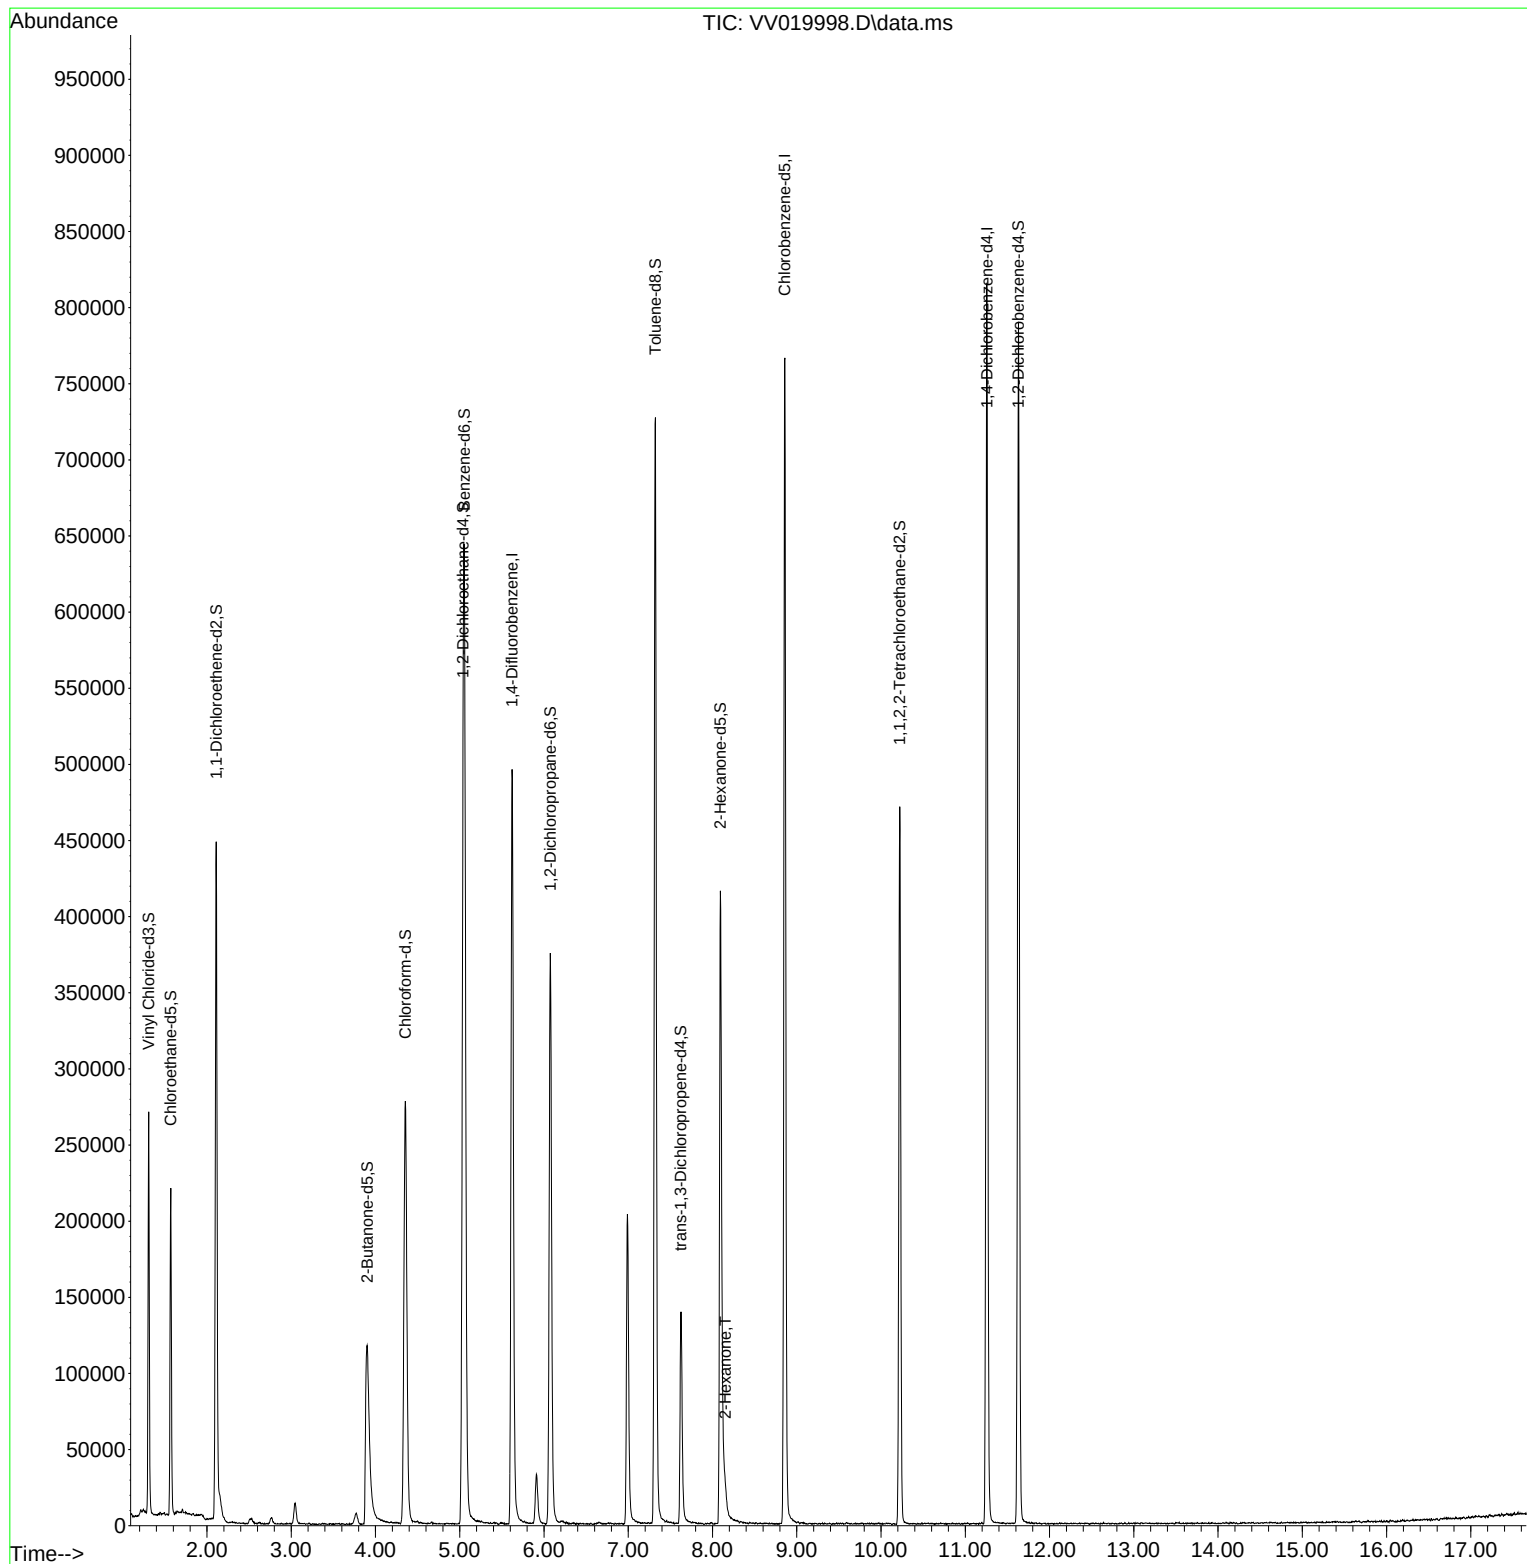

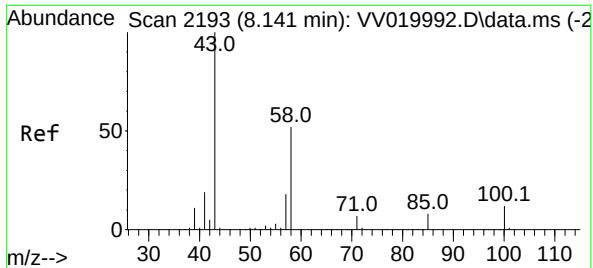

#48
 2-Hexanone
 Concen: 3.32 ug/L
 RT: 8.151 min Scan# 2196
 Delta R.T. 0.010 min
 Lab File: VV019998.D
 Acq: 14 Jan 2021 13:35

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y1

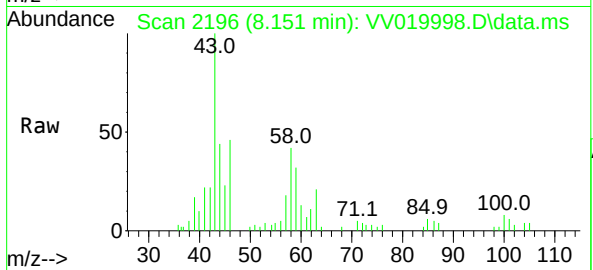

Tgt Ion: 43 Resp: 11561

Ion	Ratio	Lower	Upper
43	100		
58	40.0	41.8	62.6#
57	18.3	15.0	22.4
100	7.3	8.9	13.3#

