

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
 Data File : VV019997.D
 Acq On : 14 Jan 2021 13:12
 Operator : SY/MD
 Sample : M1147-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV019997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.306	61	67	84	rVB	259034	261797	16.08%	2.081%
2	1.566	141	148	158	rBV	212236	237614	14.60%	1.889%
3	2.106	306	316	343	rVB	438759	659329	40.50%	5.241%
4	2.688	494	497	501	rBV4	575	433	0.03%	0.003%
5	2.762	518	520	522	rBV2	552	285	0.02%	0.002%
6	2.794	526	530	532	rBV	809	522	0.03%	0.004%
7	2.830	537	541	542	rBV2	858	614	0.04%	0.005%
8	2.859	548	550	552	rBV2	591	319	0.02%	0.003%
9	2.939	568	575	577	rBV6	701	706	0.04%	0.006%
10	3.045	605	608	612	rBV4	613	427	0.03%	0.003%
11	3.212	659	660	662	rBV	491	214	0.01%	0.002%
12	3.251	670	672	674	rBV2	686	251	0.02%	0.002%
13	3.331	695	697	699	rBV3	491	320	0.02%	0.003%
14	3.418	722	724	730	rVB2	557	343	0.02%	0.003%
15	3.479	741	743	745	rBV2	382	187	0.01%	0.001%
16	3.537	758	761	762	rBV2	433	252	0.02%	0.002%
17	3.585	773	776	779	rBV	683	549	0.03%	0.004%
18	3.659	797	799	801	rBV3	671	428	0.03%	0.003%
19	3.692	807	809	812	rVB2	636	388	0.02%	0.003%
20	3.717	812	817	820	rBV3	614	732	0.04%	0.006%
21	3.791	838	840	843	rBV2	395	221	0.01%	0.002%
22	3.827	849	851	854	rBV	422	282	0.02%	0.002%
23	3.849	854	858	861	rBV3	497	468	0.03%	0.004%
24	3.894	861	872	910	rBV	110113	350112	21.51%	2.783%
25	4.351	999	1014	1048	rBV	273063	668300	41.06%	5.313%
26	4.659	1108	1110	1112	rBV2	585	336	0.02%	0.003%
27	4.753	1136	1139	1143	rVV5	953	568	0.03%	0.005%
28	4.788	1147	1150	1152	rBV2	645	352	0.02%	0.003%
29	4.897	1179	1184	1185	rBV3	838	713	0.04%	0.006%
30	4.978	1205	1209	1211	rBV4	817	578	0.04%	0.005%
31	5.048	1214	1231	1261	rBV2	631206	1627816	100.00%	12.940%
32	5.383	1331	1335	1337	rBV3	1219	783	0.05%	0.006%
33	5.515	1375	1376	1379	rBV2	509	288	0.02%	0.002%
34	5.569	1391	1393	1395	rBV3	459	240	0.01%	0.002%
35	5.621	1395	1409	1435	rBV	494000	983285	60.41%	7.816%
36	5.910	1488	1499	1518	rVB2	30235	65778	4.04%	0.523%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011421\
 Data File : VW019997.D
 Acq On : 14 Jan 2021 13:12
 Operator : SY/MD
 Sample : M1147-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.978	1518	1520	1525	rVB4	875	496	0.03%	0.004%
38	6.074	1535	1550	1575	rBV	369671	746694	45.87%	5.936%
39	6.325	1626	1628	1630	rVB3	788	358	0.02%	0.003%
40	6.338	1630	1632	1635	rBV2	513	201	0.01%	0.002%
41	6.351	1635	1636	1637	rBV	637	182	0.01%	0.001%
42	6.383	1643	1646	1650	rBV4	777	645	0.04%	0.005%
43	6.405	1650	1653	1658	rVB4	870	724	0.04%	0.006%
44	6.431	1658	1661	1667	rBV4	640	605	0.04%	0.005%
45	6.531	1689	1692	1693	rBV	355	192	0.01%	0.002%
46	6.643	1725	1727	1728	rBV	771	285	0.02%	0.002%
47	6.711	1747	1748	1751	rBV	333	183	0.01%	0.001%
48	6.762	1762	1764	1767	rBV3	691	460	0.03%	0.004%
49	6.810	1777	1779	1781	rBV2	502	179	0.01%	0.001%
50	6.917	1808	1812	1813	rBV3	597	405	0.02%	0.003%
51	6.990	1823	1835	1860	rBV2	199935	366392	22.51%	2.913%
52	7.235	1909	1911	1916	rBV5	1115	876	0.05%	0.007%
53	7.318	1926	1937	1955	rBV	716518	1237858	76.04%	9.840%
54	7.540	2003	2006	2010	rVB5	1043	712	0.04%	0.006%
55	7.624	2021	2032	2058	rBV	134293	244047	14.99%	1.940%
56	7.871	2107	2109	2111	rBV3	654	364	0.02%	0.003%
57	7.945	2130	2132	2133	rBV2	603	235	0.01%	0.002%
58	8.093	2168	2178	2219	rBV2	372648	752726	46.24%	5.984%
59	8.688	2360	2363	2366	rBV3	613	444	0.03%	0.004%
60	8.855	2404	2415	2437	rBV	740275	1214761	74.63%	9.657%
61	9.077	2481	2484	2487	rBV6	1376	984	0.06%	0.008%
62	9.116	2492	2496	2502	rBV7	1395	1760	0.11%	0.014%
63	9.270	2539	2544	2550	rBV4	777	911	0.06%	0.007%
64	9.299	2550	2553	2556	rVB3	438	250	0.02%	0.002%
65	9.322	2558	2560	2562	rBV	462	215	0.01%	0.002%
66	9.373	2574	2576	2577	rVV2	819	280	0.02%	0.002%
67	9.418	2588	2590	2594	rBV2	548	423	0.03%	0.003%
68	9.624	2650	2654	2656	rBV4	803	451	0.03%	0.004%
69	9.682	2670	2672	2674	rBV3	574	242	0.01%	0.002%
70	9.720	2682	2684	2687	rBV3	412	210	0.01%	0.002%
71	9.740	2687	2690	2691	rBV3	621	374	0.02%	0.003%
72	9.820	2713	2715	2716	rBV	467	215	0.01%	0.002%
73	9.900	2737	2740	2744	rBV4	509	425	0.03%	0.003%
74	10.132	2811	2812	2815	rBV2	575	219	0.01%	0.002%
75	10.222	2828	2840	2864	rVB	445048	696749	42.80%	5.539%
76	10.405	2895	2897	2899	rVB	631	176	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
 Data File : VV019997.D
 Acq On : 14 Jan 2021 13:12
 Operator : SY/MD
 Sample : M1147-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.450	2906	2911	2914	rBV5	884	1039	0.06%	0.008%
78	10.537	2937	2938	2943	rBV3	505	287	0.02%	0.002%
79	10.559	2943	2945	2951	rVV6	730	500	0.03%	0.004%
80	10.701	2986	2989	2993	rBV4	727	550	0.03%	0.004%
81	10.736	2998	3000	3002	rBV3	460	223	0.01%	0.002%
82	10.897	3047	3050	3052	rBV2	747	472	0.03%	0.004%
83	11.122	3119	3120	3123	rBV2	344	226	0.01%	0.002%
84	11.167	3132	3134	3137	rVB3	1101	581	0.04%	0.005%
85	11.254	3150	3161	3181	rBV	797796	1237594	76.03%	9.838%
86	11.521	3239	3244	3245	rBV2	612	462	0.03%	0.004%
87	11.550	3251	3253	3254	rBV2	526	223	0.01%	0.002%
88	11.579	3260	3262	3264	rBV3	725	440	0.03%	0.003%
89	11.630	3267	3278	3296	rVV	765119	1191525	73.20%	9.472%
90	11.804	3326	3332	3333	rBV5	1132	1157	0.07%	0.009%
91	11.897	3358	3361	3362	rBV	675	344	0.02%	0.003%
92	11.948	3375	3377	3379	rBV3	563	211	0.01%	0.002%
93	12.090	3419	3421	3422	rBV3	521	225	0.01%	0.002%
94	12.254	3469	3472	3477	rVB4	1148	824	0.05%	0.007%
95	12.276	3477	3479	3480	rBV	515	291	0.02%	0.002%
96	12.945	3685	3687	3688	rBV2	695	284	0.02%	0.002%
97	13.347	3808	3812	3813	rBV	583	404	0.02%	0.003%
98	13.389	3823	3825	3832	rBV3	778	658	0.04%	0.005%
99	13.694	3915	3920	3923	rBV3	749	820	0.05%	0.007%
100	13.926	3989	3992	3995	rBV2	768	571	0.04%	0.005%




Sum of corrected areas: 12579649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV019997.D
Acq On : 14 Jan 2021 13:12
Operator : SY/MD
Sample : M1147-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

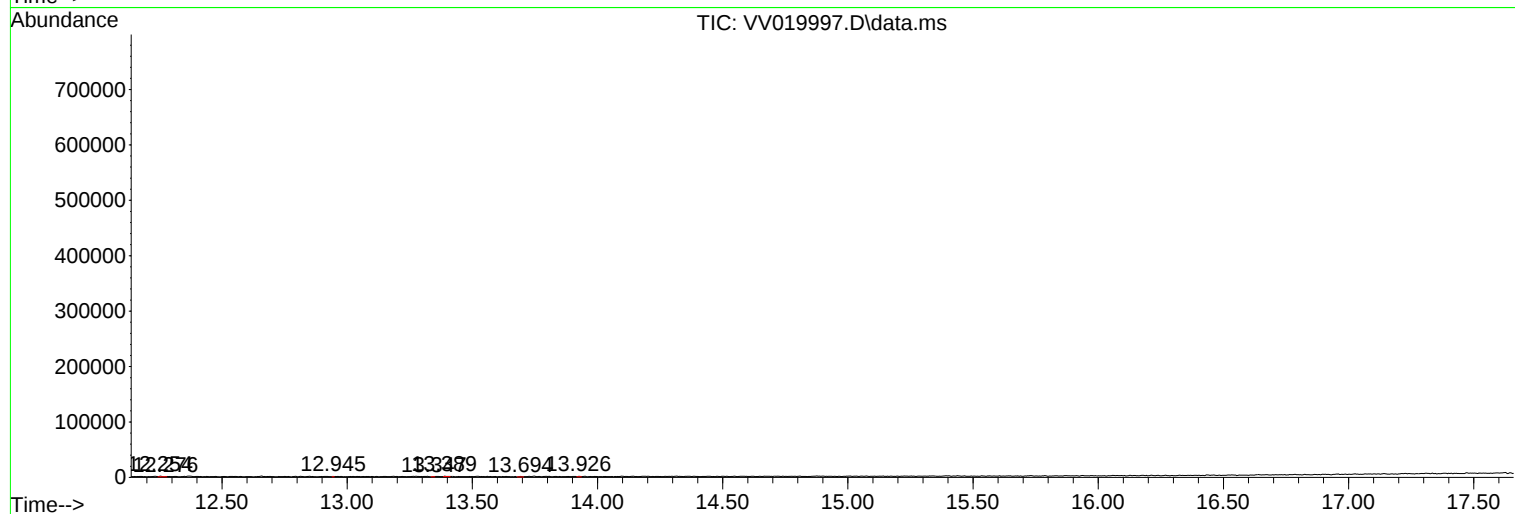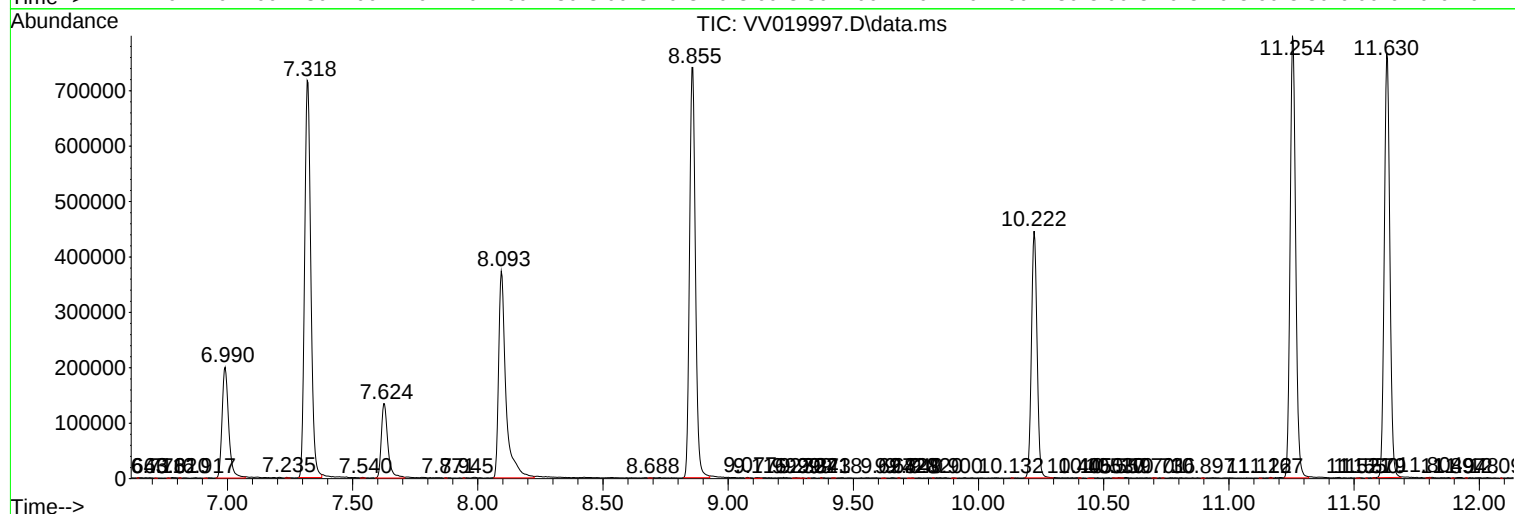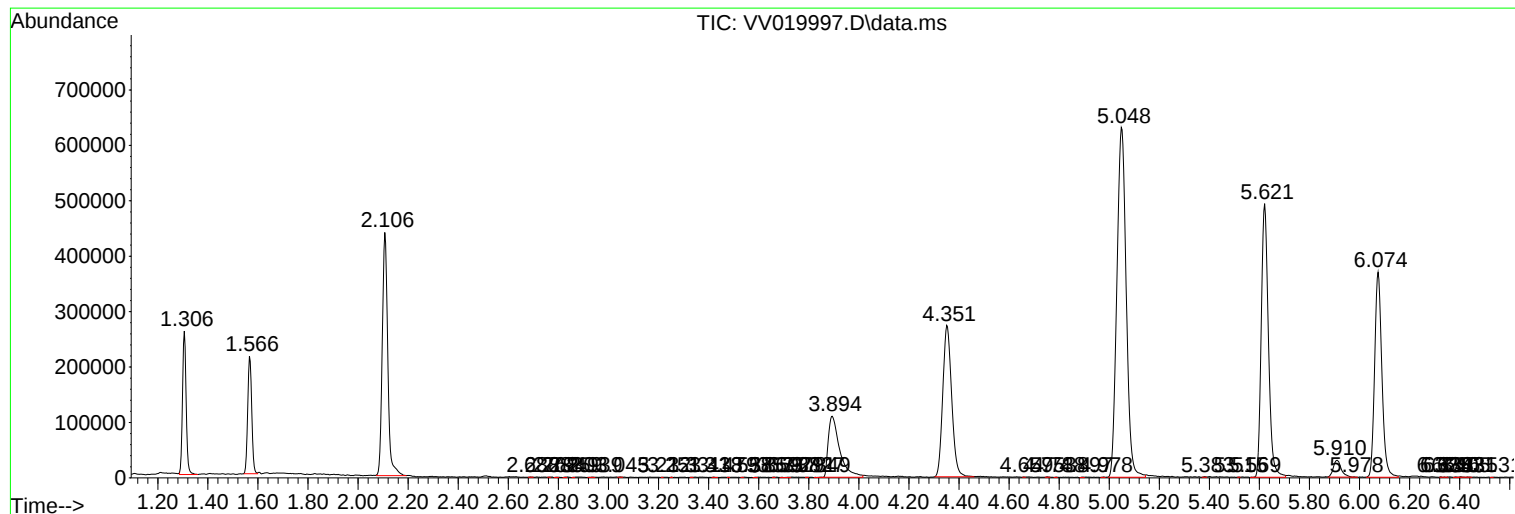

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV019997.D
Acq On : 14 Jan 2021 13:12
Operator : SY/MD
Sample : M1147-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV019997.D
Acq On : 14 Jan 2021 13:12
Operator : SY/MD
Sample : M1147-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------