

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
 Data File : VV019999.D
 Acq On : 14 Jan 2021 13:59
 Operator : SY/MD
 Sample : M1147-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV019999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	87	rVB	260934	263639	15.68%	2.073%
2	1.570	142	149	164	rVB	213591	238783	14.20%	1.878%
3	2.110	307	317	347	rVB	440539	674335	40.10%	5.303%
4	2.312	379	380	385	rVB2	832	494	0.03%	0.004%
5	2.582	461	464	466	rBV2	636	351	0.02%	0.003%
6	2.705	499	502	508	rBV4	539	612	0.04%	0.005%
7	2.740	511	513	515	rBV2	580	302	0.02%	0.002%
8	2.869	550	553	556	rVB3	732	436	0.03%	0.003%
9	2.885	556	558	560	rBV2	726	338	0.02%	0.003%
10	2.962	576	582	586	rBV4	799	725	0.04%	0.006%
11	2.987	586	590	591	rBV2	454	253	0.02%	0.002%
12	3.274	677	679	681	rVB4	687	238	0.01%	0.002%
13	3.309	687	690	692	rBV2	976	502	0.03%	0.004%
14	3.335	696	698	703	rVB3	770	547	0.03%	0.004%
15	3.360	703	706	707	rBV	444	272	0.02%	0.002%
16	3.457	732	736	737	rBV2	602	342	0.02%	0.003%
17	3.496	743	748	749	rBV3	684	493	0.03%	0.004%
18	3.557	764	767	770	rBV3	505	410	0.02%	0.003%
19	3.589	773	777	779	rBV4	681	536	0.03%	0.004%
20	3.637	790	792	794	rBV3	476	243	0.01%	0.002%
21	3.659	794	799	800	rBV3	564	318	0.02%	0.003%
22	3.836	850	854	856	rBV2	566	338	0.02%	0.003%
23	3.897	861	873	906	rBV2	115310	363323	21.61%	2.857%
24	4.354	1000	1015	1042	rVB	272199	665354	39.57%	5.232%
25	4.643	1102	1105	1109	rBV2	763	660	0.04%	0.005%
26	4.836	1162	1165	1168	rBV4	650	526	0.03%	0.004%
27	4.881	1173	1179	1181	rBV2	957	914	0.05%	0.007%
28	4.926	1185	1193	1198	rBV7	939	1096	0.07%	0.009%
29	4.971	1203	1207	1209	rBV3	488	256	0.02%	0.002%
30	4.987	1209	1212	1214	rBV	357	237	0.01%	0.002%
31	5.052	1214	1232	1267	rBV2	638673	1681509	100.00%	13.223%
32	5.309	1309	1312	1316	rBV3	968	808	0.05%	0.006%
33	5.621	1396	1409	1430	rBV	477425	958727	57.02%	7.539%
34	5.910	1490	1499	1518	rVB	31877	65838	3.92%	0.518%
35	6.074	1534	1550	1577	rBV	377574	756723	45.00%	5.951%
36	6.347	1632	1635	1637	rBV2	655	495	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
 Data File : VV019999.D
 Acq On : 14 Jan 2021 13:59
 Operator : SY/MD
 Sample : M1147-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.399	1646	1651	1653	rBV5	861	778	0.05%	0.006%
38	6.447	1664	1666	1670	rBV3	582	429	0.03%	0.003%
39	6.470	1671	1673	1676	rVV4	593	307	0.02%	0.002%
40	6.737	1753	1756	1761	rVB3	749	588	0.03%	0.005%
41	6.901	1804	1807	1809	rBV2	649	360	0.02%	0.003%
42	6.991	1824	1835	1860	rVV	199804	362640	21.57%	2.852%
43	7.241	1911	1913	1917	rBV2	471	361	0.02%	0.003%
44	7.273	1920	1923	1925	rBV2	716	517	0.03%	0.004%
45	7.322	1925	1938	1965	rBV	718041	1252905	74.51%	9.853%
46	7.579	2016	2018	2022	rVB4	844	553	0.03%	0.004%
47	7.627	2022	2033	2056	rBV	137524	245407	14.59%	1.930%
48	7.987	2136	2145	2153	rBV	1778	2533	0.15%	0.020%
49	8.055	2164	2166	2167	rBV	591	274	0.02%	0.002%
50	8.093	2168	2178	2215	rBV2	398445	785100	46.69%	6.174%
51	8.495	2301	2303	2305	rBV3	931	521	0.03%	0.004%
52	8.527	2312	2313	2315	rBV2	540	297	0.02%	0.002%
53	8.605	2333	2337	2339	rBV3	985	745	0.04%	0.006%
54	8.711	2368	2370	2373	rBV3	898	531	0.03%	0.004%
55	8.772	2387	2389	2391	rBV3	835	394	0.02%	0.003%
56	8.804	2396	2399	2401	rBV3	841	458	0.03%	0.004%
57	8.855	2401	2415	2438	rBV	729234	1194760	71.05%	9.396%
58	9.068	2479	2481	2488	rBV6	685	541	0.03%	0.004%
59	9.106	2490	2493	2494	rBV2	615	313	0.02%	0.002%
60	9.209	2522	2525	2527	rVV3	535	353	0.02%	0.003%
61	9.302	2550	2554	2555	rBV2	629	350	0.02%	0.003%
62	9.518	2619	2621	2623	rBV2	501	260	0.02%	0.002%
63	9.553	2630	2632	2633	rBV2	415	237	0.01%	0.002%
64	9.576	2635	2639	2643	rVB3	491	410	0.02%	0.003%
65	9.669	2666	2668	2669	rBV2	541	259	0.02%	0.002%
66	9.756	2691	2695	2699	rBV4	642	497	0.03%	0.004%
67	9.801	2707	2709	2712	rVB3	663	369	0.02%	0.003%
68	9.997	2768	2770	2776	rBV3	818	920	0.05%	0.007%
69	10.068	2790	2792	2797	rVB3	748	408	0.02%	0.003%
70	10.090	2797	2799	2802	rVB3	535	367	0.02%	0.003%
71	10.116	2802	2807	2809	rBV3	732	489	0.03%	0.004%
72	10.142	2813	2815	2818	rVB3	941	325	0.02%	0.003%
73	10.161	2818	2821	2825	rBV3	620	511	0.03%	0.004%
74	10.222	2828	2840	2857	rBV	460781	716206	42.59%	5.632%
75	10.396	2891	2894	2896	rBV2	763	380	0.02%	0.003%
76	10.437	2902	2907	2912	rBV4	595	715	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
 Data File : VV019999.D
 Acq On : 14 Jan 2021 13:59
 Operator : SY/MD
 Sample : M1147-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.463	2912	2915	2918	rVV3	407	338	0.02%	0.003%
78	10.553	2941	2943	2945	rBV3	620	334	0.02%	0.003%
79	10.659	2973	2976	2979	rBV4	503	400	0.02%	0.003%
80	10.778	3010	3013	3014	rBV2	734	442	0.03%	0.003%
81	10.878	3041	3044	3045	rBV2	852	471	0.03%	0.004%
82	10.994	3076	3080	3082	rBV4	473	367	0.02%	0.003%
83	11.084	3104	3108	3113	rBV4	689	707	0.04%	0.006%
84	11.122	3117	3120	3122	rVB3	486	267	0.02%	0.002%
85	11.177	3135	3137	3141	rVB	461	270	0.02%	0.002%
86	11.196	3141	3143	3148	rBV4	549	450	0.03%	0.004%
87	11.254	3150	3161	3181	rBV	796534	1226812	72.96%	9.648%
88	11.630	3266	3278	3299	rBV	788339	1224409	72.82%	9.629%
89	12.145	3434	3438	3442	rVB4	774	665	0.04%	0.005%
90	12.305	3486	3488	3497	rVB5	930	873	0.05%	0.007%
91	12.344	3498	3500	3502	rBV	524	294	0.02%	0.002%
92	12.469	3536	3539	3540	rBV2	537	259	0.02%	0.002%
93	12.514	3550	3553	3556	rBV2	830	637	0.04%	0.005%
94	12.810	3643	3645	3646	rBV2	638	252	0.01%	0.002%
95	12.894	3668	3671	3673	rBV2	619	361	0.02%	0.003%
96	12.965	3690	3693	3697	rBV4	681	475	0.03%	0.004%
97	13.215	3768	3771	3774	rBV4	624	578	0.03%	0.005%
98	13.643	3902	3904	3906	rBV	615	378	0.02%	0.003%
99	13.730	3928	3931	3933	rBV3	642	406	0.02%	0.003%
100	13.775	3943	3945	3948	rBV2	841	471	0.03%	0.004%




Sum of corrected areas: 12716257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV019999.D
Acq On : 14 Jan 2021 13:59
Operator : SY/MD
Sample : M1147-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

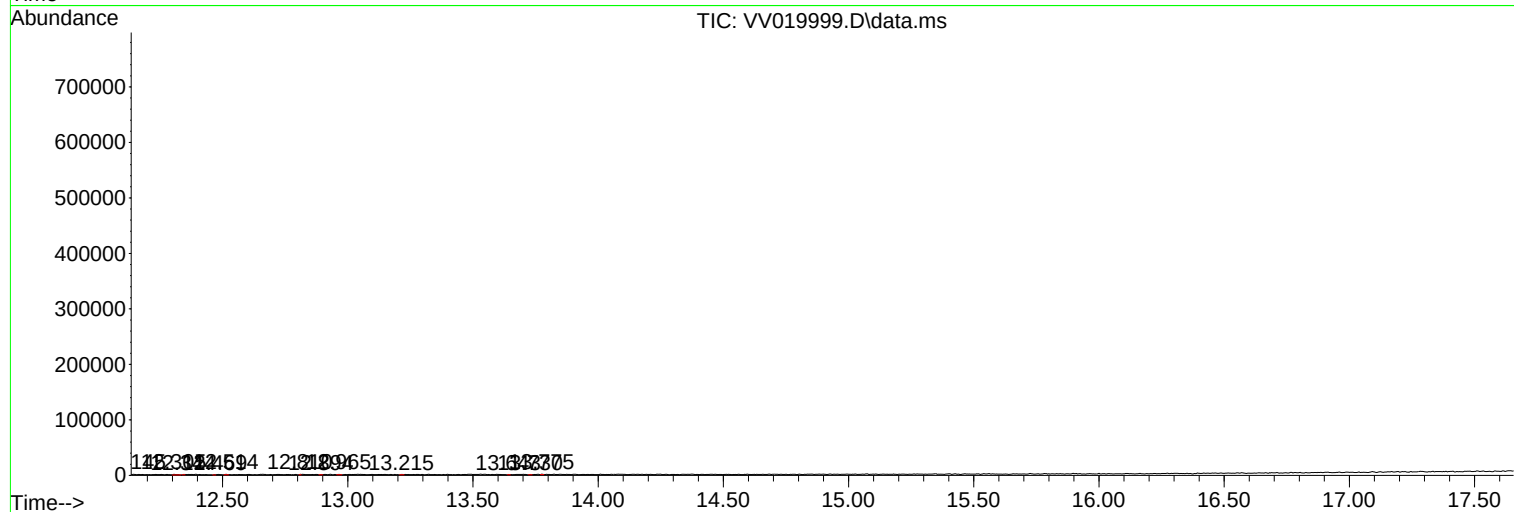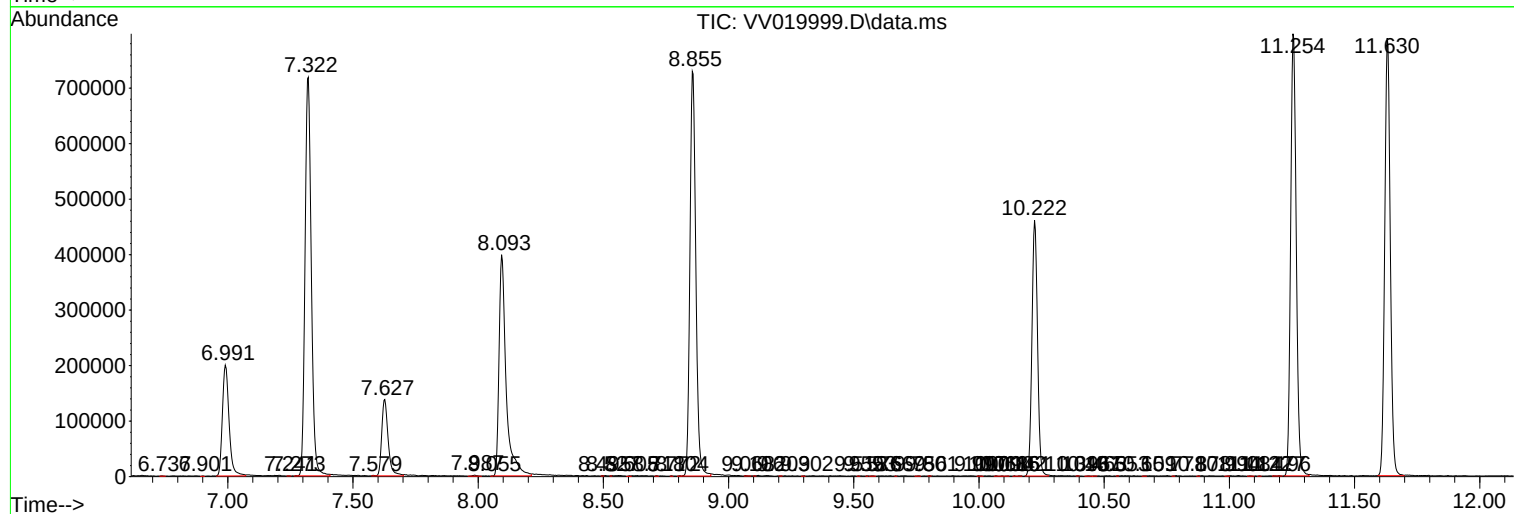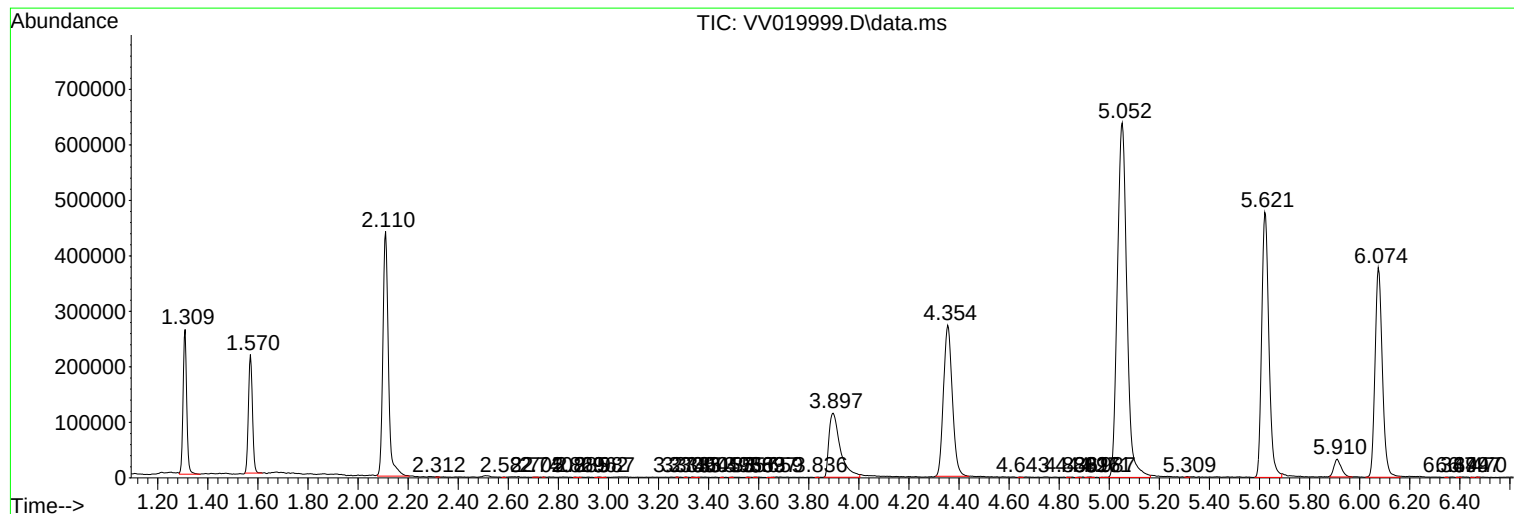

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV019999.D
Acq On : 14 Jan 2021 13:59
Operator : SY/MD
Sample : M1147-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV019999.D
Acq On : 14 Jan 2021 13:59
Operator : SY/MD
Sample : M1147-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
