
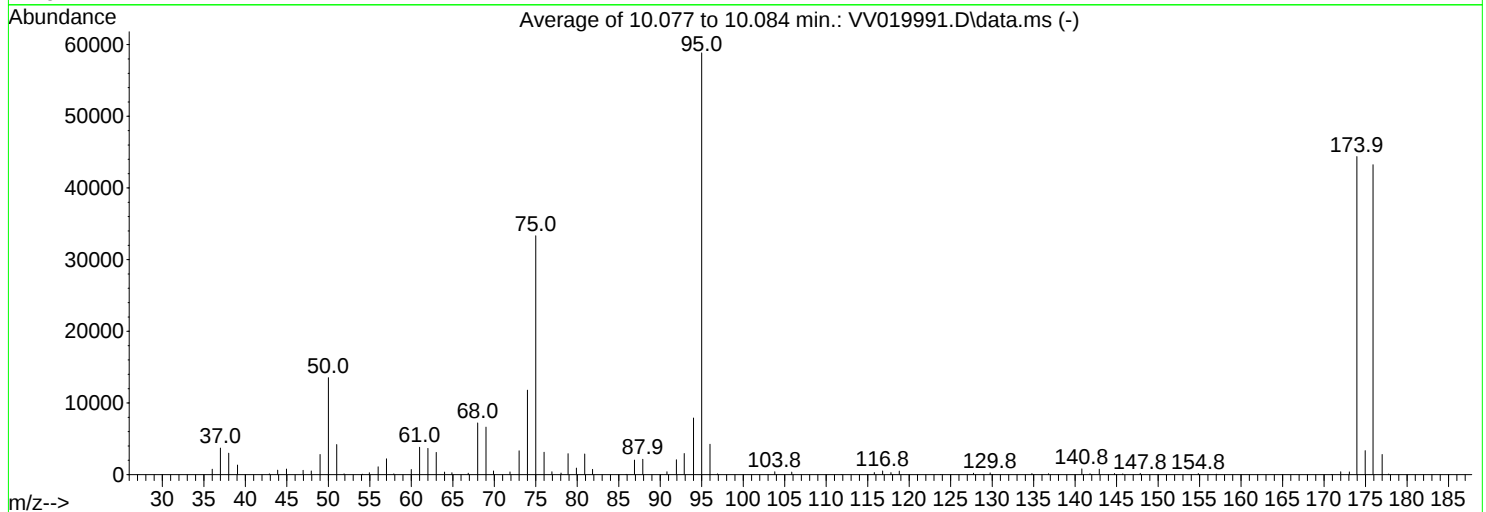


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011421\
Data File : VV01991.D
Acq On : 14 Jan 2021 09:04
Operator : SY/MD
Sample : BFB80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB80

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM011121WMA.M
Title : VOC Analysis
Last Update : Sat Jan 16 04:43:48 2021

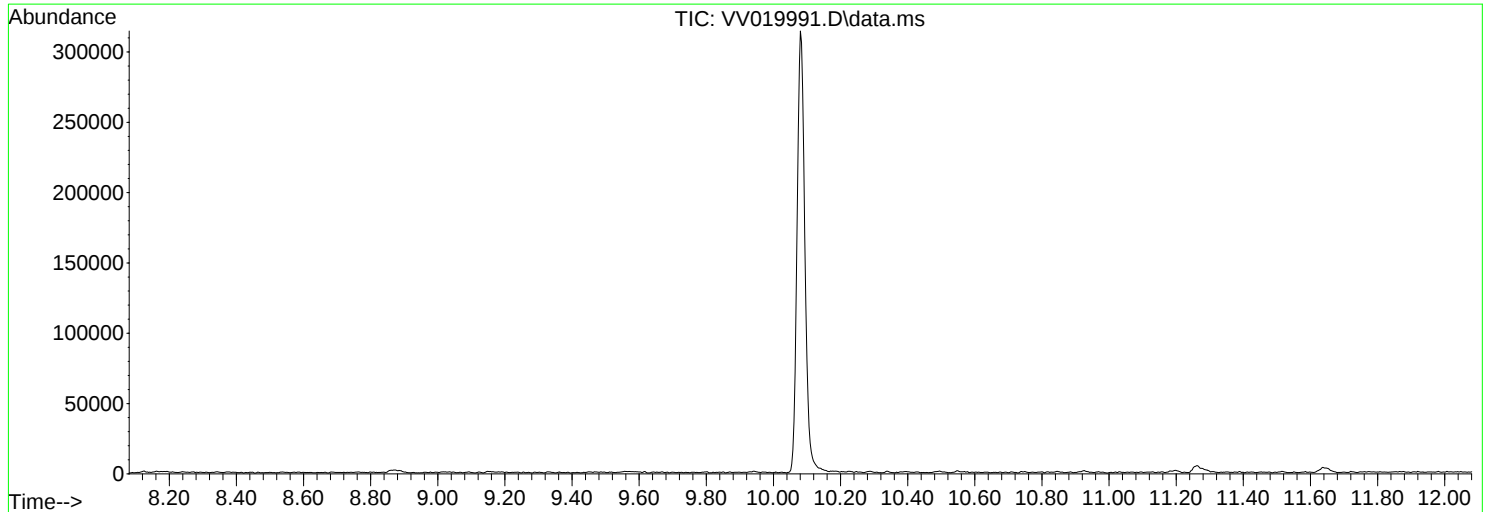

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	13526	PASS
75	95	30	80	56.6	33323	PASS
95	95	100	100	100.0	58853	PASS
96	95	5	9	7.2	4252	PASS
173	174	0.00	2	0.8	370	PASS
174	95	50	120	75.4	44376	PASS
175	174	5	9	7.5	3349	PASS
176	174	95	101	97.5	43253	PASS
177	176	5	9	6.5	2817	PASS

m/z	Abundance
37.00	106.0
39.90	235.0
43.90	535.0
51.80	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	822.0
37.00	3688.0
38.00	2913.0
39.00	1345.0
40.00	212.0
42.90	131.0
43.90	1138.0
44.90	759.0
46.90	585.0
47.90	525.0
49.00	2912.0
50.00	13443.0
51.00	3971.0
52.00	257.0
54.90	186.0
56.00	995.0
57.00	2145.0
60.00	748.0
61.00	3661.0
62.00	3285.0
63.00	3053.0
64.00	386.0
64.90	254.0
66.80	188.0
68.00	6804.0
69.00	6614.0
69.90	477.0
71.90	331.0
73.00	3279.0
74.00	11282.0
75.00	32376.0
76.00	3129.0
76.90	360.0
78.10	223.0
78.90	2858.0
79.90	868.0
80.90	2712.0
81.90	666.0
85.90	120.0
86.90	1858.0
87.90	2116.0
90.80	408.0
92.00	1998.0
92.90	2963.0
94.00	7442.0
95.00	55848.0
96.00	4153.0
96.90	118.0
103.80	374.0
105.90	355.0
115.80	304.0
116.80	429.0
117.80	315.0
118.80	453.0
127.70	202.0
128.90	108.0
129.80	298.0
134.80	116.0
136.80	118.0
140.80	808.0
141.80	171.0
142.90	689.0
144.70	134.0
145.80	111.0
147.80	159.0
154.90	126.0
157.10	111.0
172.00	416.0
173.00	531.0
173.90	42024.0
174.90	3275.0
175.90	40512.0
177.00	2744.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	793.0
37.00	3959.0
38.00	3071.0
39.10	1335.0
39.90	227.0
42.90	130.0
43.90	1183.0
45.00	794.0
46.90	650.0
47.90	520.0
49.00	2873.0
50.00	13968.0
51.00	4373.0
52.00	204.0
54.10	100.0
55.00	275.0
56.00	1133.0
57.00	2344.0
57.90	138.0
60.00	728.0
61.00	3999.0
62.00	3826.0
63.00	3257.0
64.00	394.0
64.90	273.0
66.90	194.0
68.00	7475.0
69.00	6773.0
69.90	549.0
71.90	386.0
73.00	3462.0
74.00	12222.0
75.00	34448.0
76.00	3267.0
77.00	405.0
78.00	218.0
78.90	3024.0
79.90	988.0
80.90	2976.0
81.90	765.0
86.90	2011.0
87.90	2196.0
90.80	420.0
92.00	2165.0
92.90	3034.0
94.00	8154.0
95.00	60648.0
96.00	4422.0
96.90	104.0
103.80	416.0
105.80	381.0
111.80	103.0
115.80	316.0
116.80	523.0
117.80	314.0
118.80	510.0
127.70	224.0
129.70	237.0
134.80	134.0
136.80	130.0
140.80	809.0
141.80	150.0
142.90	802.0
144.80	173.0
145.80	119.0
147.90	183.0
154.80	157.0
157.00	120.0
170.90	106.0
172.00	439.0
173.10	579.0
173.90	45752.0
175.00	3514.0
175.90	44840.0
177.00	2914.0
177.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	688.0
37.00	3771.0
38.00	2979.0
39.10	1364.0
39.90	250.0
42.90	106.0
43.90	1144.0
45.00	762.0
47.00	610.0
48.00	484.0
49.00	2669.0
50.00	13167.0
51.00	4257.0
52.00	156.0
54.10	107.0
54.90	322.0
56.00	1182.0
57.00	2143.0
57.90	178.0
60.00	693.0
61.00	3788.0
62.00	3856.0
63.00	3011.0
64.00	303.0
64.90	284.0
66.90	207.0
68.00	7355.0
69.00	6493.0
69.90	543.0
71.90	403.0
73.00	3238.0
74.00	11879.0
75.00	33144.0
76.00	3000.0
77.00	415.0
78.00	259.0
78.90	2907.0
79.90	924.0
80.90	2931.0
81.80	769.0
86.90	2196.0
87.90	2093.0
90.80	391.0
91.90	2036.0
92.90	2819.0
94.00	8091.0
95.00	60064.0
96.00	4181.0
96.90	104.0
103.80	394.0
105.80	355.0
115.80	282.0
116.80	570.0
117.80	276.0
118.80	539.0
123.80	100.0
127.80	200.0
129.70	191.0
134.80	208.0
136.80	148.0
140.80	800.0
141.80	103.0
142.90	810.0
144.80	201.0
145.60	104.0
147.90	187.0
154.80	186.0
172.00	376.0
174.00	45352.0
175.00	3259.0
175.90	44408.0
177.00	2792.0
177.80	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80