

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011521\
Data File : VW020018.D
Acq On : 15 Jan 2021 12:14
Operator : SY/MD
Sample : M1147-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T5

Manual Integrations
APPROVED

MMDadoda
1/18/2021 12:48:37 PM

Quant Time: Jan 16 04:44:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jan 16 04:43:48 2021
Response via : Initial Calibration

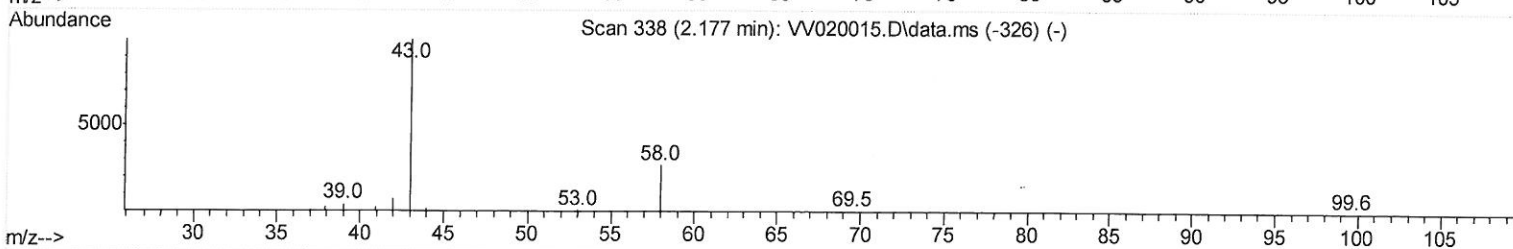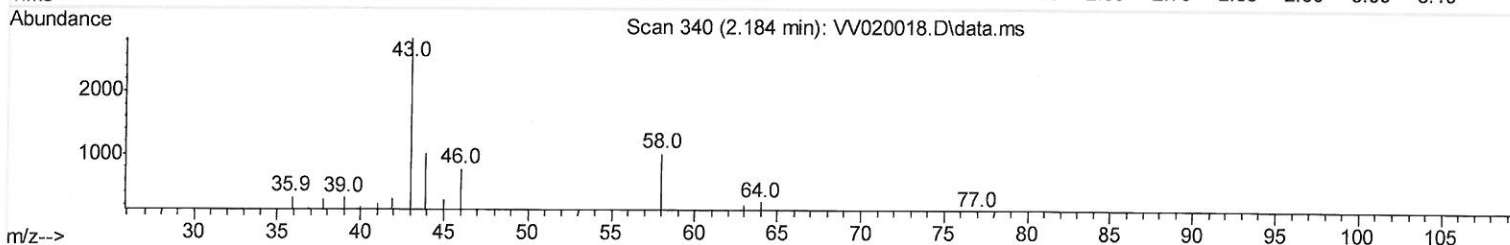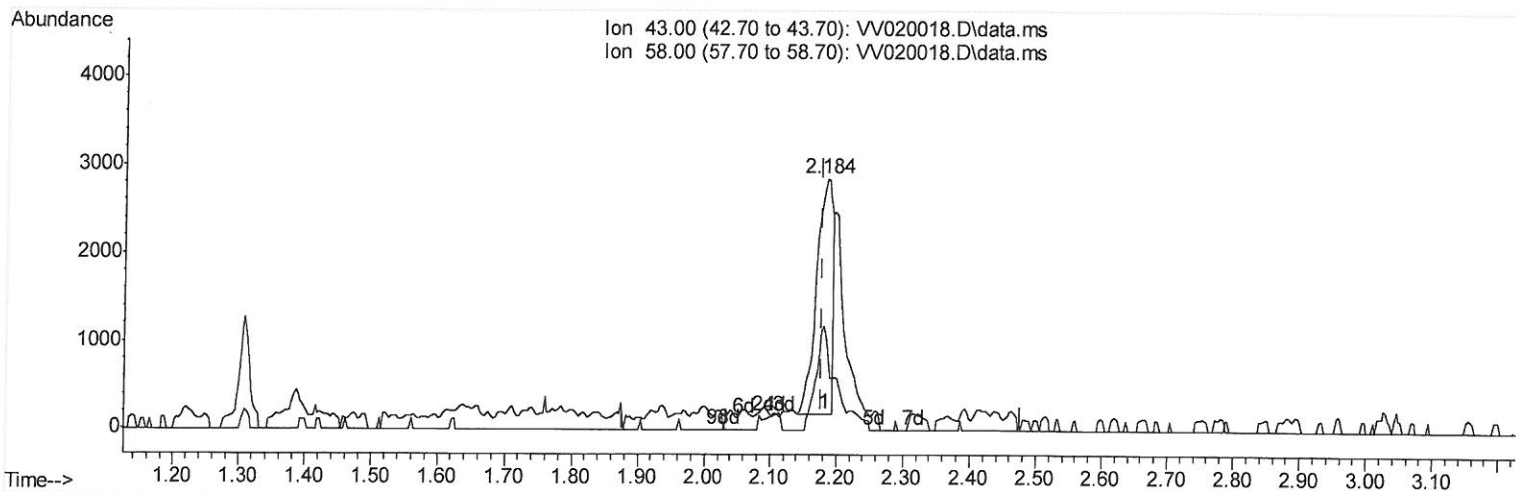

TIC: VW020018.D\data.ms

(13) Acetone (T)

2.184min (+ 0.006) 2.46 ug/L

response 4562

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.10	35.44
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020018.D
Acq On : 15 Jan 2021 12:14
Operator : SY/MD
Sample : M1147-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T5

Manual Integrations
APPROVED

MMDadoda
1/18/2021 12:48:37 PM

Quant Time: Jan 16 04:44:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jan 16 04:43:48 2021
Response via : Initial Calibration

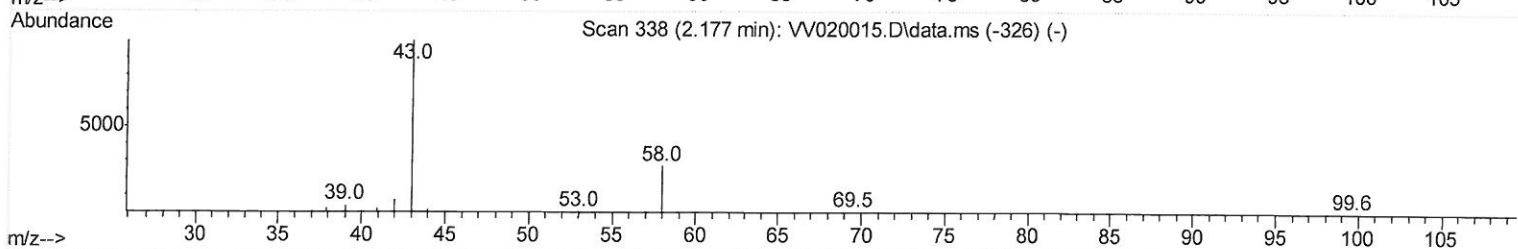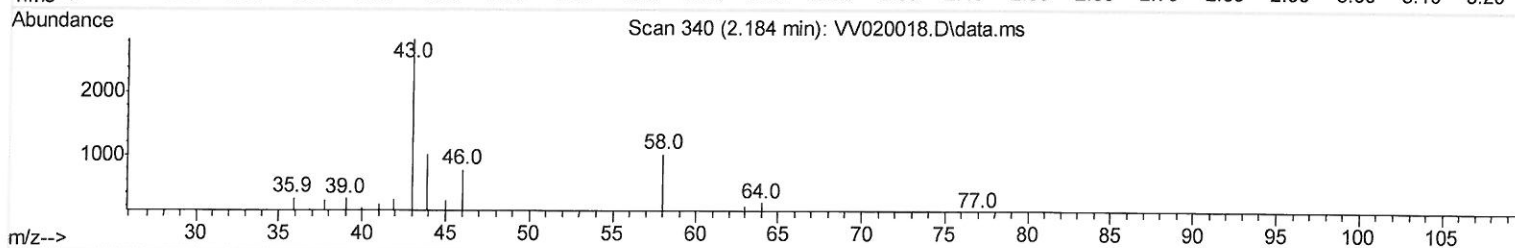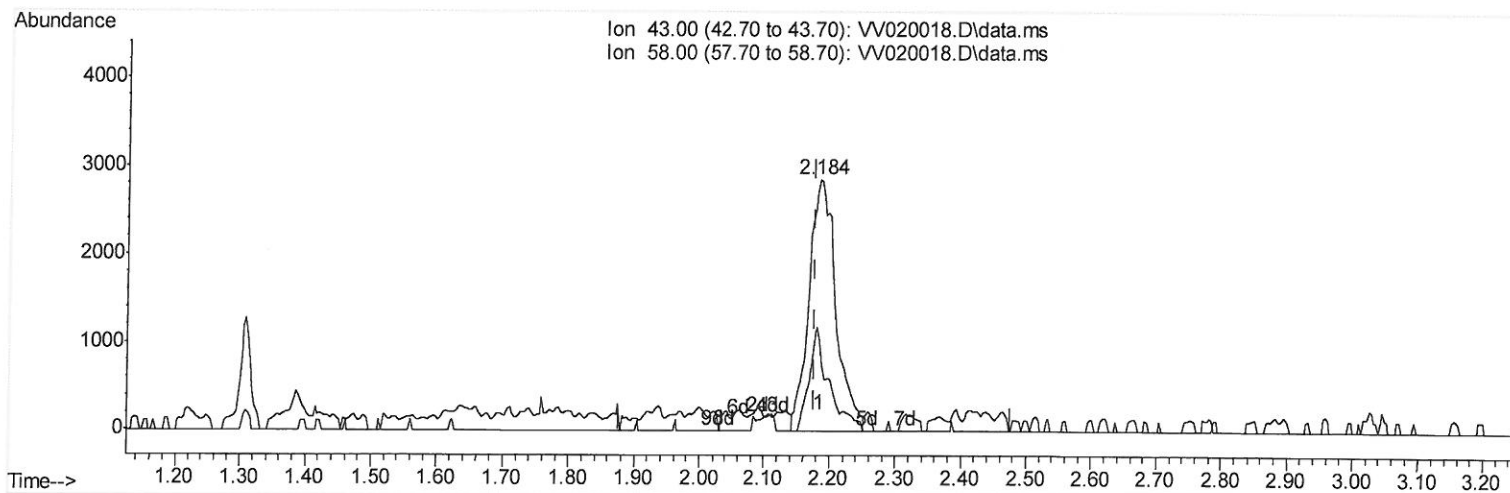

TIC: VV020018.D\data.ms

(13) Acetone (T)

2.184min (+ 0.006) 4.38 ug/L m

response 8118

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.10	19.92
0.00	0.00	0.00
0.00	0.00	0.00

> 1/25/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\W011521\
 Data File : W020018.D
 Acq On : 15 Jan 2021 12:14
 Operator : SY/MD
 Sample : M1147-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 BG4T5

Manual Integrations
 APPROVED

MMDadoda
 1/18/2021 12:48:37 PM

Quant Time: Jan 16 04:44:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jan 16 04:43:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.617	114	383092	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.855	117	370555	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.254	152	187358	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	134811	41.72	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.44%		
7) Chloroethane-d5	1.569	69	120197	46.60	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.20%		
11) 1,1-Dichloroethene-d2	2.106	63	217528	34.18	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.36%		
21) 2-Butanone-d5	3.888	46	176376	84.14	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.14%		
24) Chloroform-d	4.347	84	245589	42.19	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.38%		
26) 1,2-Dichloroethane-d4	5.032	65	180092	45.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.02%		
32) Benzene-d6	5.052	84	457245	43.72	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.44%		
36) 1,2-Dichloropropane-d6	6.071	67	145669	44.61	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.22%		
41) Toluene-d8	7.318	98	403678	42.59	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.18%		
43) trans-1,3-Dichloroprop...	7.624	79	66325	39.14	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.28%		
47) 2-Hexanone-d5	8.090	63	92186	70.42	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	70.42%		
57) 1,1,2,2-Tetrachloroeth...	10.222	84	168612	38.20	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	76.40%		
64) 1,2-Dichlorobenzene-d4	11.630	152	166591	46.04	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.08%		
Target Compounds						
13) Acetone	2.184	43	8118m	4.38	ug/L	
48) 2-Hexanone	8.145	43	17227	5.11	ug/L #	68

Qvalue

#

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011521\
Data File : VW020018.D
Acq On : 15 Jan 2021 12:14
Operator : SY/MD
Sample : M1147-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4T5

Manual Integrations
APPROVED

MMDadoda
1/18/2021 12:48:37 PM

Quant Time: Jan 16 04:44:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jan 16 04:43:48 2021
Response via : Initial Calibration

