

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020017.D
 Acq On : 15 Jan 2021 11:24
 Operator : SY/MD
 Sample : VV0115WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020017.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	201714	208162	13.76%	1.757%
2	1.569	142	149	165	rBV	190862	216486	14.31%	1.828%
3	2.110	307	317	347	rVB	380472	592135	39.13%	4.999%
4	2.299	368	376	381	rBV8	2006	3488	0.23%	0.029%
5	2.421	412	414	422	rBV4	1024	1122	0.07%	0.009%
6	2.897	559	562	565	rVB3	749	515	0.03%	0.004%
7	3.023	598	601	603	rVB2	766	348	0.02%	0.003%
8	3.036	603	605	610	rBV4	668	641	0.04%	0.005%
9	3.209	656	659	661	rVB	705	369	0.02%	0.003%
10	3.245	664	670	672	rBV5	861	925	0.06%	0.008%
11	3.299	683	687	688	rBV3	693	423	0.03%	0.004%
12	3.338	696	699	701	rBV3	564	353	0.02%	0.003%
13	3.521	754	756	758	rBV2	477	320	0.02%	0.003%
14	3.598	777	780	782	rBV3	628	437	0.03%	0.004%
15	3.685	803	807	810	rBV3	958	537	0.04%	0.005%
16	3.820	845	849	852	rBV2	797	592	0.04%	0.005%
17	3.894	861	872	908	rBV	109010	338980	22.40%	2.862%
18	4.354	1000	1015	1042	rBV	252136	618985	40.91%	5.226%
19	4.698	1118	1122	1126	rBV4	916	812	0.05%	0.007%
20	4.759	1139	1141	1148	rBV3	1009	1109	0.07%	0.009%
21	4.952	1199	1201	1205	rBV3	657	477	0.03%	0.004%
22	5.052	1213	1232	1265	rBV2	582326	1513205	100.00%	12.775%
23	5.453	1354	1357	1361	rVB4	993	717	0.05%	0.006%
24	5.492	1365	1369	1374	rVV6	1141	1331	0.09%	0.011%
25	5.621	1397	1409	1434	rVV	467620	931664	61.57%	7.865%
26	5.910	1486	1499	1514	rBV4	33127	71172	4.70%	0.601%
27	5.987	1521	1523	1526	rBV3	990	533	0.04%	0.004%
28	6.074	1537	1550	1574	rBV2	343680	696083	46.00%	5.876%
29	6.273	1611	1612	1616	rVB2	924	409	0.03%	0.003%
30	6.376	1639	1644	1646	rBV4	974	731	0.05%	0.006%
31	6.569	1702	1704	1706	rBV4	778	331	0.02%	0.003%
32	6.598	1710	1713	1715	rBV2	512	378	0.02%	0.003%
33	6.659	1730	1732	1735	rVB3	860	343	0.02%	0.003%
34	6.743	1755	1758	1761	rVB4	712	495	0.03%	0.004%
35	6.884	1798	1802	1804	rBV2	576	425	0.03%	0.004%
36	6.920	1809	1813	1815	rBV	601	569	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020017.D
 Acq On : 15 Jan 2021 11:24
 Operator : SY/MD
 Sample : VV0115WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.990	1824	1835	1859	rBV	183629	337359	22.29%	2.848%
38	7.322	1926	1938	1959	rBV	654748	1136200	75.09%	9.592%
39	7.627	2023	2033	2055	rBV	126646	223003	14.74%	1.883%
40	7.826	2092	2095	2097	rBV3	754	619	0.04%	0.005%
41	7.949	2130	2133	2137	rBV3	664	464	0.03%	0.004%
42	8.093	2167	2178	2214	rBV2	354252	720325	47.60%	6.081%
43	8.621	2339	2342	2345	rBV3	692	507	0.03%	0.004%
44	8.659	2352	2354	2356	rBV	663	362	0.02%	0.003%
45	8.682	2360	2361	2365	rVV2	753	323	0.02%	0.003%
46	8.775	2388	2390	2392	rBV2	944	501	0.03%	0.004%
47	8.858	2403	2416	2437	rBV	725583	1175157	77.66%	9.921%
48	9.209	2521	2525	2528	rBV2	914	688	0.05%	0.006%
49	9.331	2560	2563	2566	rBV3	676	530	0.04%	0.004%
50	9.411	2585	2588	2591	rVB4	1031	598	0.04%	0.005%
51	9.431	2591	2594	2596	rBV2	692	423	0.03%	0.004%
52	9.444	2596	2598	2603	rVB2	914	606	0.04%	0.005%
53	9.473	2603	2607	2610	rBV4	700	513	0.03%	0.004%
54	9.592	2641	2644	2645	rBV3	977	565	0.04%	0.005%
55	9.801	2706	2709	2711	rBV3	470	330	0.02%	0.003%
56	9.852	2721	2725	2727	rVB2	453	327	0.02%	0.003%
57	9.881	2729	2734	2737	rBV4	436	479	0.03%	0.004%
58	9.977	2760	2764	2767	rBV3	890	652	0.04%	0.006%
59	10.000	2769	2771	2775	rBV2	754	351	0.02%	0.003%
60	10.019	2775	2777	2780	rBV2	569	421	0.03%	0.004%
61	10.074	2792	2794	2798	rVB3	672	337	0.02%	0.003%
62	10.119	2805	2808	2810	rBV4	440	322	0.02%	0.003%
63	10.222	2828	2840	2858	rBV	425643	674370	44.57%	5.693%
64	10.373	2884	2887	2890	rBV2	803	708	0.05%	0.006%
65	10.450	2906	2911	2913	rBV5	690	692	0.05%	0.006%
66	10.505	2923	2928	2932	rBV3	633	604	0.04%	0.005%
67	10.546	2937	2941	2943	rBV4	530	463	0.03%	0.004%
68	10.630	2964	2967	2970	rVB2	738	386	0.03%	0.003%
69	10.675	2979	2981	2984	rBV3	653	473	0.03%	0.004%
70	10.836	3027	3031	3033	rBV3	505	342	0.02%	0.003%
71	10.846	3033	3034	3038	rVB2	686	349	0.02%	0.003%
72	10.926	3054	3059	3060	rBV4	891	764	0.05%	0.006%
73	10.964	3068	3071	3073	rBV	528	339	0.02%	0.003%
74	11.103	3110	3114	3116	rBV3	998	616	0.04%	0.005%
75	11.257	3150	3162	3182	rBV	777149	1195928	79.03%	10.096%
76	11.485	3230	3233	3236	rVB3	721	407	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020017.D
 Acq On : 15 Jan 2021 11:24
 Operator : SY/MD
 Sample : VV0115WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	11.556	3253	3255	3258	rBV2	606	356	0.02%	0.003%
78	11.630	3266	3278	3298	rBV	734364	1148657	75.91%	9.697%
79	11.810	3331	3334	3336	rBV2	750	411	0.03%	0.003%
80	11.890	3357	3359	3364	rBV3	688	674	0.04%	0.006%
81	11.919	3366	3368	3371	rVV2	688	324	0.02%	0.003%
82	12.180	3446	3449	3451	rBV3	564	395	0.03%	0.003%
83	12.215	3457	3460	3462	rBV2	686	351	0.02%	0.003%
84	12.366	3504	3507	3508	rBV2	798	401	0.03%	0.003%
85	12.447	3529	3532	3536	rVV5	736	617	0.04%	0.005%
86	12.656	3592	3597	3599	rBV4	1823	1484	0.10%	0.013%
87	12.694	3605	3609	3611	rBV2	587	550	0.04%	0.005%
88	12.717	3614	3616	3619	rVV2	670	333	0.02%	0.003%
89	12.775	3632	3634	3638	rBV5	505	363	0.02%	0.003%
90	12.852	3655	3658	3661	rBV3	893	462	0.03%	0.004%
91	12.871	3661	3664	3667	rBV4	770	623	0.04%	0.005%
92	13.013	3705	3708	3711	rVB3	781	552	0.04%	0.005%
93	13.029	3711	3713	3716	rBV	531	339	0.02%	0.003%
94	13.276	3786	3790	3793	rBV4	1344	1251	0.08%	0.011%
95	13.312	3799	3801	3805	rBV2	552	347	0.02%	0.003%
96	13.524	3863	3867	3870	rBV5	1255	1036	0.07%	0.009%
97	13.607	3888	3893	3896	rVB3	954	721	0.05%	0.006%
98	13.624	3896	3898	3901	rBV3	707	469	0.03%	0.004%
99	13.932	3992	3994	3997	rBV2	600	366	0.02%	0.003%
100	14.794	4260	4262	4264	rBV2	831	358	0.02%	0.003%




Sum of corrected areas: 11845445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020017.D
Acq On : 15 Jan 2021 11:24
Operator : SY/MD
Sample : VV0115WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

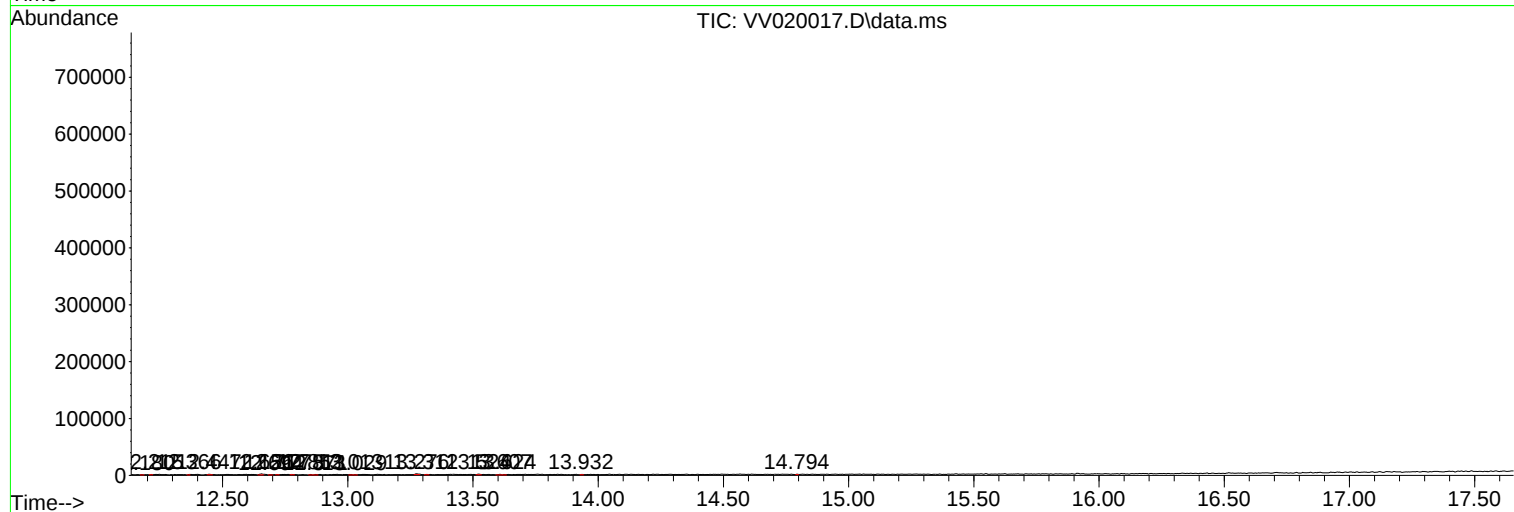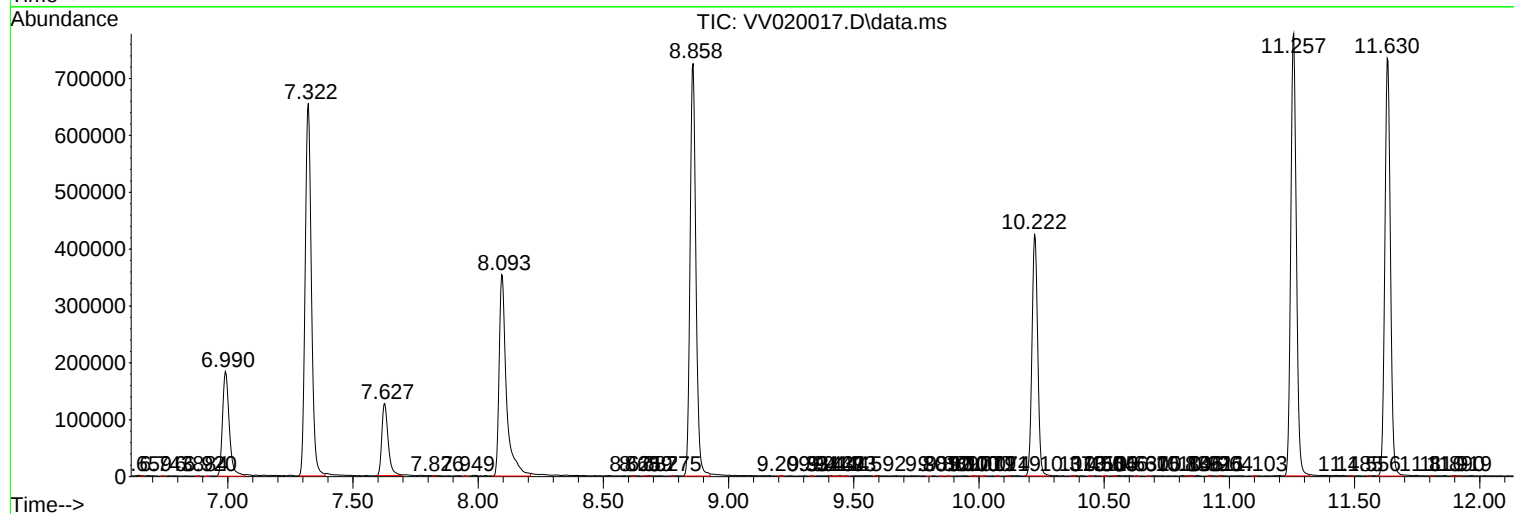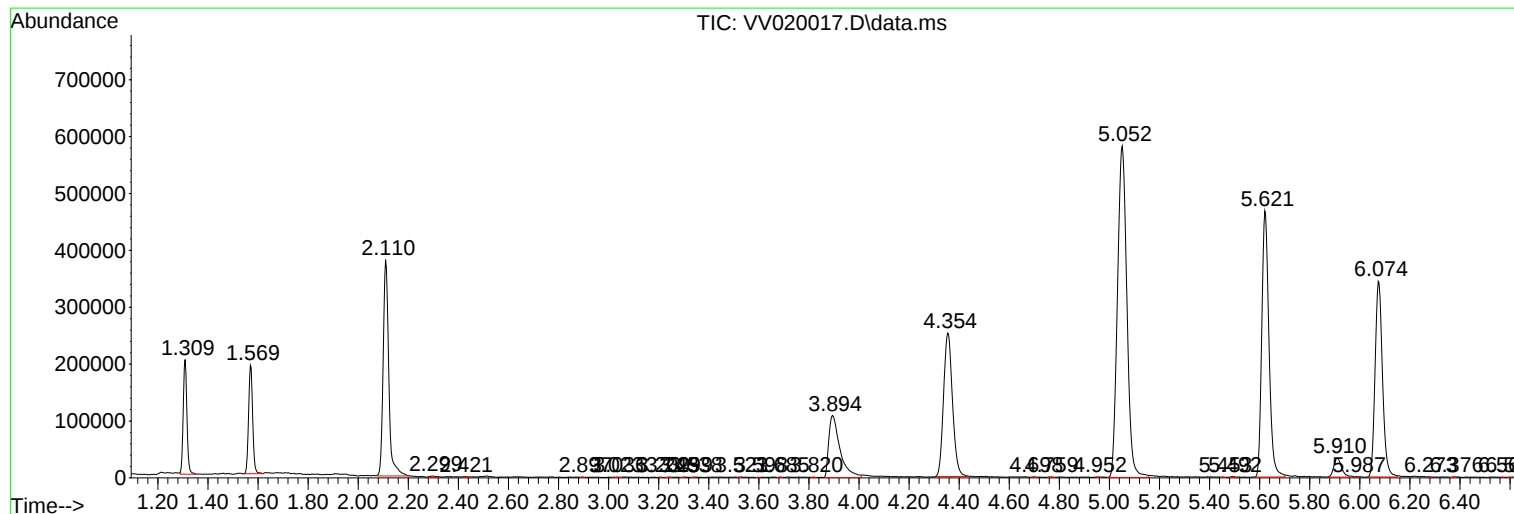

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020017.D
Acq On : 15 Jan 2021 11:24
Operator : SY/MD
Sample : VV0115WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020017.D
Acq On : 15 Jan 2021 11:24
Operator : SY/MD
Sample : VV0115WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
