

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020021.D
 Acq On : 15 Jan 2021 13:24
 Operator : SY/MD
 Sample : M1147-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB	228114	239352	15.09%	1.912%
2	1.569	142	149	159	rBV	223818	239953	15.12%	1.916%
3	2.109	307	317	344	rVB	413309	636943	40.14%	5.087%
4	2.576	460	462	464	rBV3	822	412	0.03%	0.003%
5	2.701	499	501	504	rBV2	437	266	0.02%	0.002%
6	2.836	540	543	545	rVV4	901	395	0.02%	0.003%
7	2.965	579	583	587	rVB5	960	719	0.05%	0.006%
8	3.222	659	663	664	rBV3	543	347	0.02%	0.003%
9	3.244	668	670	672	rBV2	553	269	0.02%	0.002%
10	3.331	693	697	700	rBV3	723	639	0.04%	0.005%
11	3.392	713	716	717	rBV	516	252	0.02%	0.002%
12	3.460	731	737	738	rBV3	960	696	0.04%	0.006%
13	3.524	752	757	760	rVB3	610	502	0.03%	0.004%
14	3.543	760	763	764	rBV2	556	279	0.02%	0.002%
15	3.585	775	776	781	rVB4	637	429	0.03%	0.003%
16	3.621	785	787	791	rBV4	396	313	0.02%	0.002%
17	3.659	794	799	802	rBV4	775	623	0.04%	0.005%
18	3.695	808	810	812	rBV2	622	288	0.02%	0.002%
19	3.736	820	823	825	rBV3	595	437	0.03%	0.003%
20	3.759	825	830	834	rBV6	1424	2024	0.13%	0.016%
21	3.891	860	871	899	rBV2	127285	367225	23.15%	2.933%
22	4.354	998	1015	1045	rBV	265500	652905	41.15%	5.215%
23	4.566	1079	1081	1083	rBV3	841	459	0.03%	0.004%
24	4.666	1109	1112	1115	rBV3	753	561	0.04%	0.004%
25	4.717	1126	1128	1132	rBV4	472	278	0.02%	0.002%
26	4.736	1132	1134	1137	rVB4	708	398	0.03%	0.003%
27	4.891	1178	1182	1185	rBV2	875	760	0.05%	0.006%
28	5.051	1213	1232	1261	rBV2	614746	1586612	100.00%	12.672%
29	5.415	1343	1345	1347	rBV	846	395	0.02%	0.003%
30	5.531	1378	1381	1383	rVB3	925	574	0.04%	0.005%
31	5.550	1383	1387	1389	rBV4	758	644	0.04%	0.005%
32	5.621	1397	1409	1434	rBV	484347	970671	61.18%	7.752%
33	5.910	1488	1499	1516	rBV2	33041	69734	4.40%	0.557%
34	6.074	1535	1550	1577	rBV	357146	729206	45.96%	5.824%
35	6.331	1627	1630	1632	rBV3	618	352	0.02%	0.003%
36	6.489	1676	1679	1682	rBV3	599	416	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020021.D
 Acq On : 15 Jan 2021 13:24
 Operator : SY/MD
 Sample : M1147-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

37	6.508	1682	1685	1690	rVB3	608	526	0.03%	0.004%
38	6.637	1723	1725	1726	rBV2	804	381	0.02%	0.003%
39	6.691	1740	1742	1746	rVB5	964	569	0.04%	0.005%
40	6.746	1757	1759	1760	rBV	782	251	0.02%	0.002%
41	6.781	1766	1770	1772	rVB3	433	274	0.02%	0.002%
42	6.855	1791	1793	1795	rBV	548	272	0.02%	0.002%
43	6.932	1815	1817	1822	rVB3	769	590	0.04%	0.005%
44	6.990	1822	1835	1860	rBV2	192080	352831	22.24%	2.818%
45	7.270	1920	1922	1925	rVB3	962	421	0.03%	0.003%
46	7.321	1925	1938	1961	rBV	700116	1209124	76.21%	9.657%
47	7.627	2022	2033	2055	rBV	134695	238557	15.04%	1.905%
48	7.897	2115	2117	2119	rVB2	769	394	0.02%	0.003%
49	7.920	2119	2124	2126	rBV4	971	912	0.06%	0.007%
50	8.093	2166	2178	2218	rBV2	404688	816782	51.48%	6.523%
51	8.466	2292	2294	2298	rVB2	1360	673	0.04%	0.005%
52	8.518	2307	2310	2314	rBV7	638	485	0.03%	0.004%
53	8.537	2314	2316	2319	rBV3	711	338	0.02%	0.003%
54	8.617	2339	2341	2345	rBV4	674	315	0.02%	0.003%
55	8.733	2373	2377	2379	rBV3	490	421	0.03%	0.003%
56	8.858	2404	2416	2442	rBV	766519	1227841	77.39%	9.806%
57	9.186	2516	2518	2520	rBV	588	368	0.02%	0.003%
58	9.219	2526	2528	2531	rVB2	886	350	0.02%	0.003%
59	9.424	2590	2592	2598	rBV4	700	593	0.04%	0.005%
60	9.530	2621	2625	2628	rBV3	890	591	0.04%	0.005%
61	9.543	2628	2629	2634	rBV3	435	332	0.02%	0.003%
62	9.701	2674	2678	2680	rBV3	819	605	0.04%	0.005%
63	9.791	2704	2706	2709	rBV3	423	269	0.02%	0.002%
64	9.842	2718	2722	2725	rBV4	1050	958	0.06%	0.008%
65	9.997	2766	2770	2773	rBV3	428	337	0.02%	0.003%
66	10.122	2807	2809	2811	rBV3	707	269	0.02%	0.002%
67	10.222	2827	2840	2861	rBV	446897	708201	44.64%	5.656%
68	10.620	2962	2964	2969	rVB3	798	640	0.04%	0.005%
69	10.723	2995	2996	3000	rBV2	559	384	0.02%	0.003%
70	10.743	3000	3002	3005	rVV2	587	334	0.02%	0.003%
71	10.759	3005	3007	3010	rVV3	586	358	0.02%	0.003%
72	10.858	3036	3038	3044	rVB4	1032	775	0.05%	0.006%
73	10.926	3055	3059	3063	rBV5	853	675	0.04%	0.005%
74	10.961	3065	3070	3072	rBV3	674	420	0.03%	0.003%
75	11.051	3095	3098	3101	rBV3	564	454	0.03%	0.004%
76	11.141	3123	3126	3127	rBV2	632	354	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020021.D
 Acq On : 15 Jan 2021 13:24
 Operator : SY/MD
 Sample : M1147-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	11.254	3150	3161	3190	rBV	803476	1245711	78.51%	9.949%
78	11.566	3256	3258	3261	rBV3	674	378	0.02%	0.003%
79	11.630	3266	3278	3299	rVV	758170	1188590	74.91%	9.493%
80	11.784	3324	3326	3330	rVB4	1199	674	0.04%	0.005%
81	12.025	3398	3401	3403	rBV2	647	336	0.02%	0.003%
82	12.042	3403	3406	3408	rBV	688	440	0.03%	0.004%
83	12.090	3418	3421	3422	rBV3	459	250	0.02%	0.002%
84	12.135	3433	3435	3439	rBV4	564	391	0.02%	0.003%
85	12.202	3452	3456	3457	rBV2	452	316	0.02%	0.003%
86	12.321	3491	3493	3495	rBV2	415	311	0.02%	0.002%
87	12.376	3508	3510	3513	rBV3	711	408	0.03%	0.003%
88	12.572	3570	3571	3575	rVB3	880	405	0.03%	0.003%
89	12.595	3575	3578	3584	rBV4	516	445	0.03%	0.004%
90	13.090	3729	3732	3736	rBV3	761	558	0.04%	0.004%
91	13.144	3741	3749	3757	rBV6	1109	1607	0.10%	0.013%
92	13.276	3788	3790	3793	rBV2	877	603	0.04%	0.005%
93	13.363	3815	3817	3818	rBV2	690	265	0.02%	0.002%
94	13.424	3832	3836	3839	rVB6	781	567	0.04%	0.005%
95	13.440	3839	3841	3843	rBV2	595	307	0.02%	0.002%
96	13.533	3865	3870	3872	rBV5	996	913	0.06%	0.007%
97	13.797	3950	3952	3954	rBV2	633	319	0.02%	0.003%
98	14.067	4032	4036	4037	rBV	541	390	0.02%	0.003%
99	14.701	4231	4233	4235	rBV2	672	333	0.02%	0.003%
100	15.080	4349	4351	4356	rBV3	1111	773	0.05%	0.006%




Sum of corrected areas: 12520842

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020021.D
Acq On : 15 Jan 2021 13:24
Operator : SY/MD
Sample : M1147-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

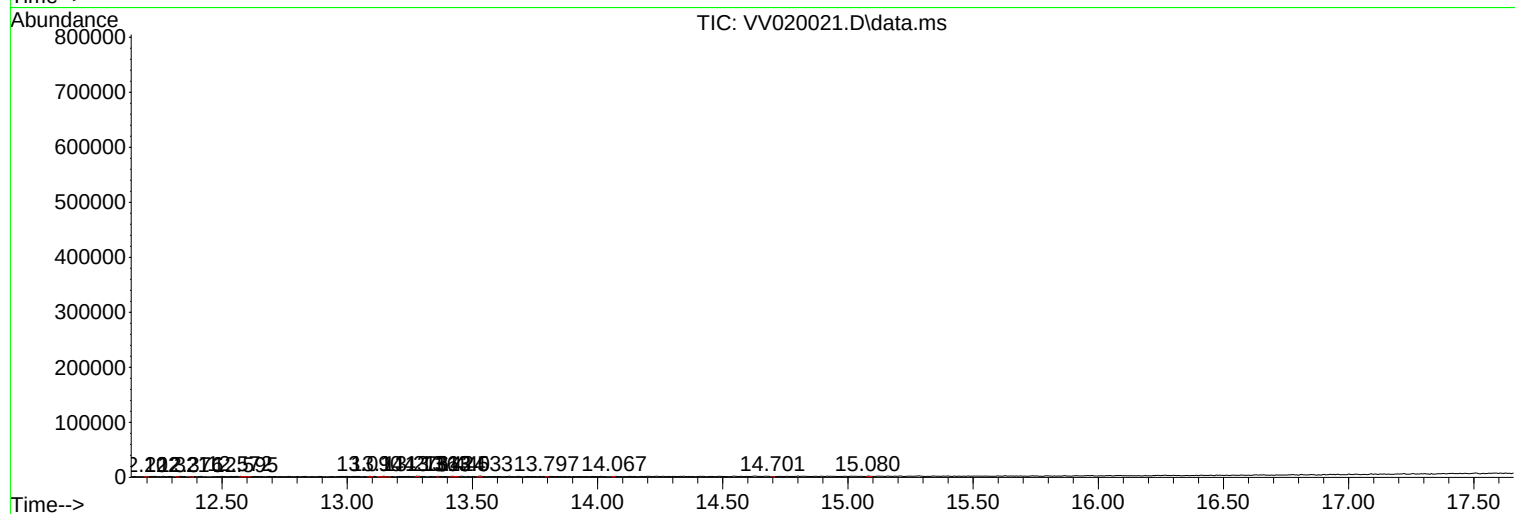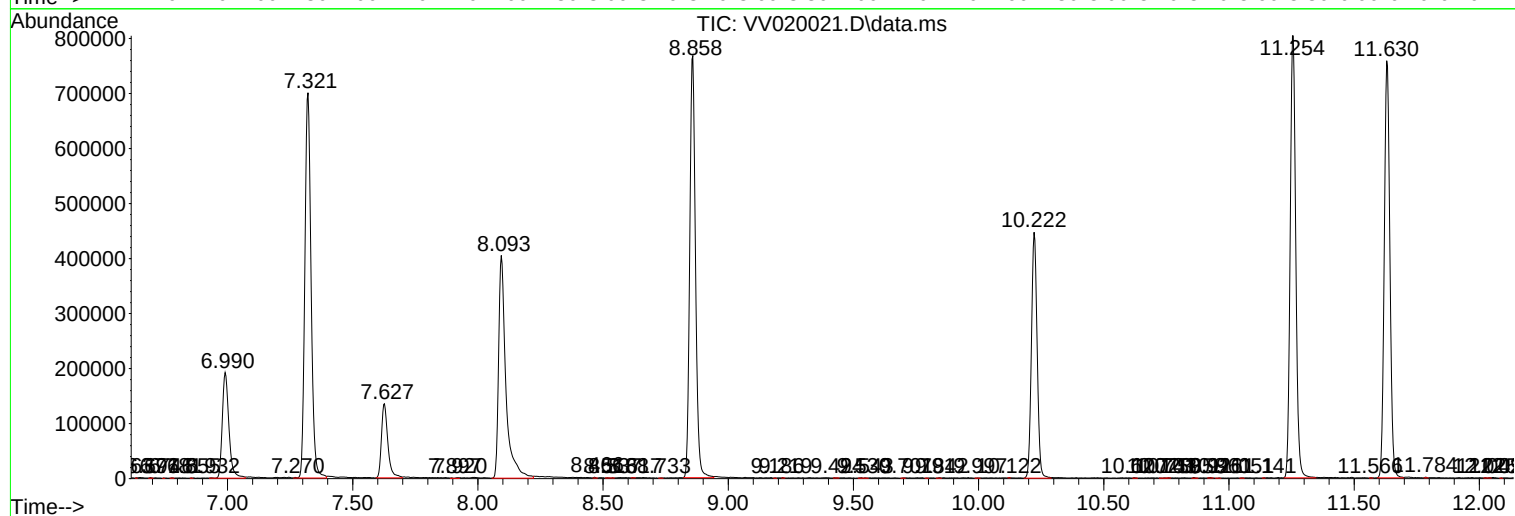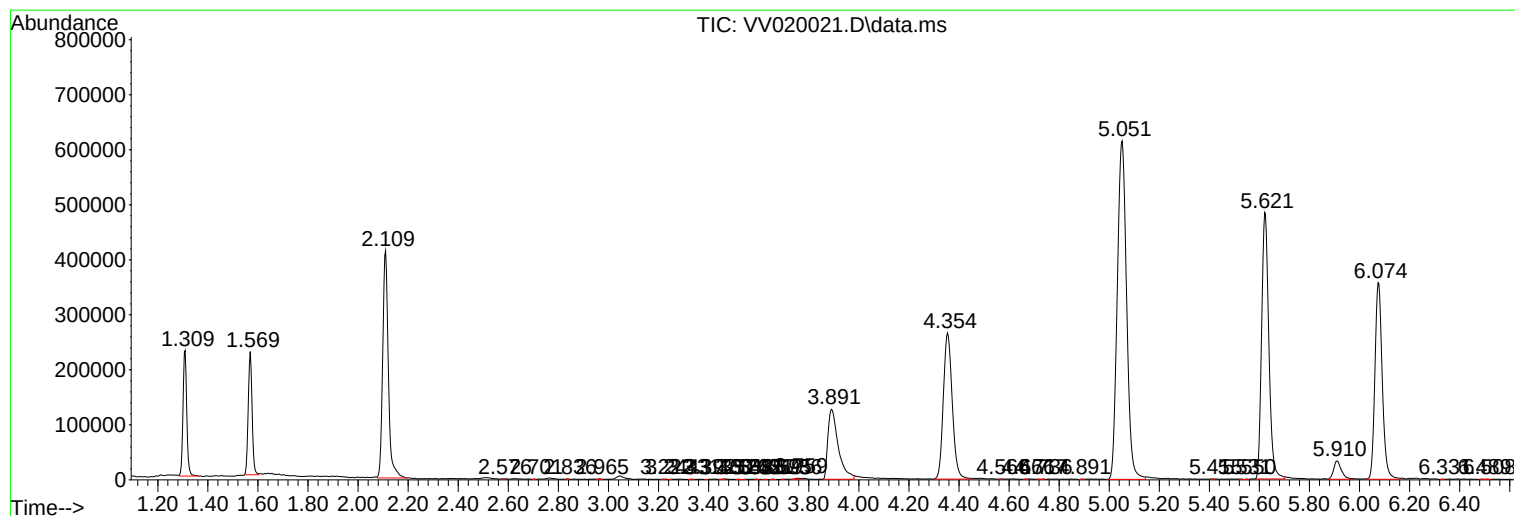

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020021.D
Acq On : 15 Jan 2021 13:24
Operator : SY/MD
Sample : M1147-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020021.D
Acq On : 15 Jan 2021 13:24
Operator : SY/MD
Sample : M1147-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
