

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020023.D
 Acq On : 15 Jan 2021 14:11
 Operator : SY/MD
 Sample : M1147-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	234603	234016	14.97%	1.901%
2	1.570	142	149	163	rVB	199891	223019	14.26%	1.812%
3	2.110	307	317	348	rVB	412997	634073	40.55%	5.151%
4	2.669	489	491	493	rBV3	750	474	0.03%	0.004%
5	2.733	506	511	512	rBV3	837	644	0.04%	0.005%
6	3.007	593	596	598	rBV2	458	268	0.02%	0.002%
7	3.045	598	608	619	rBV8	4108	8647	0.55%	0.070%
8	3.145	636	639	641	rBV2	782	519	0.03%	0.004%
9	3.200	654	656	660	rVB4	555	298	0.02%	0.002%
10	3.222	661	663	667	rVB3	842	352	0.02%	0.003%
11	3.377	707	711	714	rVV3	547	348	0.02%	0.003%
12	3.393	714	716	718	rVV2	925	444	0.03%	0.004%
13	3.531	756	759	761	rBV2	432	243	0.02%	0.002%
14	3.560	766	768	772	rVB4	639	431	0.03%	0.004%
15	3.586	772	776	777	rBV2	559	378	0.02%	0.003%
16	3.631	785	790	792	rBV3	768	628	0.04%	0.005%
17	3.647	792	795	799	rVV3	579	475	0.03%	0.004%
18	3.695	803	810	813	rVB4	727	646	0.04%	0.005%
19	3.724	813	819	822	rBV5	1251	1191	0.08%	0.010%
20	3.897	862	873	913	rBV	110332	369698	23.64%	3.003%
21	4.354	1001	1015	1045	rVB	259046	636213	40.69%	5.169%
22	4.553	1076	1077	1081	rBV3	562	256	0.02%	0.002%
23	4.585	1084	1087	1089	rBV3	923	573	0.04%	0.005%
24	4.656	1108	1109	1111	rBV2	593	256	0.02%	0.002%
25	4.804	1153	1155	1158	rVB2	494	262	0.02%	0.002%
26	4.872	1173	1176	1179	rBV4	408	389	0.02%	0.003%
27	4.975	1205	1208	1212	rBV3	511	263	0.02%	0.002%
28	5.052	1212	1232	1264	rBV2	607645	1563635	100.00%	12.703%
29	5.293	1304	1307	1312	rBV5	973	843	0.05%	0.007%
30	5.399	1339	1340	1344	rBV3	641	295	0.02%	0.002%
31	5.621	1395	1409	1437	rBV	483534	973551	62.26%	7.909%
32	5.807	1463	1467	1470	rBV5	810	679	0.04%	0.006%
33	5.827	1470	1473	1479	rVV5	895	1031	0.07%	0.008%
34	5.910	1487	1499	1517	rBV4	32545	71454	4.57%	0.580%
35	6.074	1535	1550	1574	rBV	350156	718782	45.97%	5.839%
36	6.335	1629	1631	1634	rVB3	803	430	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020023.D
 Acq On : 15 Jan 2021 14:11
 Operator : SY/MD
 Sample : M1147-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	6.392	1647	1649	1653	rVB3	621	275	0.02%	0.002%
38	6.418	1653	1657	1664	rBV4	965	1178	0.08%	0.010%
39	6.454	1666	1668	1670	rVB	686	321	0.02%	0.003%
40	6.595	1709	1712	1713	rBV	568	300	0.02%	0.002%
41	6.614	1716	1718	1721	rBV4	468	353	0.02%	0.003%
42	6.791	1771	1773	1777	rBV2	543	433	0.03%	0.004%
43	6.888	1800	1803	1804	rBV2	660	341	0.02%	0.003%
44	6.942	1816	1820	1822	rBV3	617	475	0.03%	0.004%
45	6.990	1823	1835	1859	rBV	189192	344115	22.01%	2.796%
46	7.122	1874	1876	1881	rVB4	1137	554	0.04%	0.005%
47	7.193	1896	1898	1902	rBV3	948	722	0.05%	0.006%
48	7.322	1926	1938	1971	rBV	692331	1192876	76.29%	9.691%
49	7.627	2021	2033	2062	rBV2	130637	237548	15.19%	1.930%
50	7.900	2112	2118	2120	rBV4	1118	918	0.06%	0.007%
51	7.987	2141	2145	2149	rVB5	991	1078	0.07%	0.009%
52	8.039	2158	2161	2162	rBV2	516	262	0.02%	0.002%
53	8.093	2168	2178	2213	rBV2	374827	763118	48.80%	6.200%
54	8.634	2339	2346	2348	rBV7	973	863	0.06%	0.007%
55	8.646	2348	2350	2351	rBV2	648	287	0.02%	0.002%
56	8.855	2403	2415	2439	rBV	746260	1221421	78.11%	9.923%
57	9.145	2503	2505	2506	rBV	916	404	0.03%	0.003%
58	9.183	2515	2517	2527	rBV8	611	803	0.05%	0.007%
59	9.312	2555	2557	2562	rVB3	714	495	0.03%	0.004%
60	9.498	2611	2615	2619	rBV3	835	656	0.04%	0.005%
61	9.572	2636	2638	2640	rVB	669	253	0.02%	0.002%
62	9.588	2640	2643	2644	rBV2	633	339	0.02%	0.003%
63	9.672	2667	2669	2670	rBV2	589	235	0.02%	0.002%
64	9.804	2707	2710	2712	rBV4	864	328	0.02%	0.003%
65	9.817	2712	2714	2718	rVB3	557	250	0.02%	0.002%
66	9.891	2734	2737	2739	rBV2	505	237	0.02%	0.002%
67	10.019	2771	2777	2780	rBV4	826	832	0.05%	0.007%
68	10.222	2828	2840	2859	rBV	435922	681754	43.60%	5.539%
69	10.367	2881	2885	2888	rVB3	696	427	0.03%	0.003%
70	10.431	2901	2905	2906	rBV2	1105	631	0.04%	0.005%
71	10.441	2906	2908	2911	rVB2	589	301	0.02%	0.002%
72	10.560	2942	2945	2948	rBV4	613	520	0.03%	0.004%
73	10.585	2948	2953	2955	rVB	775	537	0.03%	0.004%
74	10.601	2955	2958	2961	rBV2	599	478	0.03%	0.004%
75	10.646	2968	2972	2975	rVB3	765	542	0.03%	0.004%
76	10.768	3006	3010	3011	rBV3	1096	700	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020023.D
 Acq On : 15 Jan 2021 14:11
 Operator : SY/MD
 Sample : M1147-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

77	10.794	3016	3018	3021	rVB2	646	376	0.02%	0.003%
78	11.138	3121	3125	3128	rBV3	606	515	0.03%	0.004%
79	11.164	3128	3133	3134	rBV2	471	381	0.02%	0.003%
80	11.254	3150	3161	3178	rBV	803852	1225069	78.35%	9.952%
81	11.466	3224	3227	3229	rBV2	908	630	0.04%	0.005%
82	11.543	3248	3251	3252	rBV2	600	310	0.02%	0.003%
83	11.630	3267	3278	3299	rBV	741226	1169809	74.81%	9.503%
84	11.810	3330	3334	3335	rBV4	915	611	0.04%	0.005%
85	11.855	3345	3348	3352	rVB3	857	562	0.04%	0.005%
86	12.186	3447	3451	3455	rVB3	715	617	0.04%	0.005%
87	12.209	3455	3458	3459	rBV2	738	282	0.02%	0.002%
88	12.231	3463	3465	3469	rBV2	723	520	0.03%	0.004%
89	12.357	3501	3504	3509	rBV3	620	599	0.04%	0.005%
90	12.383	3510	3512	3516	rBV3	756	516	0.03%	0.004%
91	12.463	3534	3537	3542	rVB	525	344	0.02%	0.003%
92	12.485	3542	3544	3549	rVB4	720	465	0.03%	0.004%
93	12.723	3616	3618	3621	rBV2	512	240	0.02%	0.002%
94	12.801	3638	3642	3644	rBV3	432	350	0.02%	0.003%
95	12.833	3650	3652	3655	rBV3	418	316	0.02%	0.003%
96	13.045	3716	3718	3720	rBV2	818	388	0.02%	0.003%
97	13.511	3861	3863	3866	rBV3	841	502	0.03%	0.004%
98	13.701	3919	3922	3924	rBV2	659	342	0.02%	0.003%
99	14.264	4094	4097	4101	rBV5	898	798	0.05%	0.006%
100	15.402	4448	4451	4454	rBV5	955	838	0.05%	0.007%




Sum of corrected areas: 12309244

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020023.D
Acq On : 15 Jan 2021 14:11
Operator : SY/MD
Sample : M1147-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

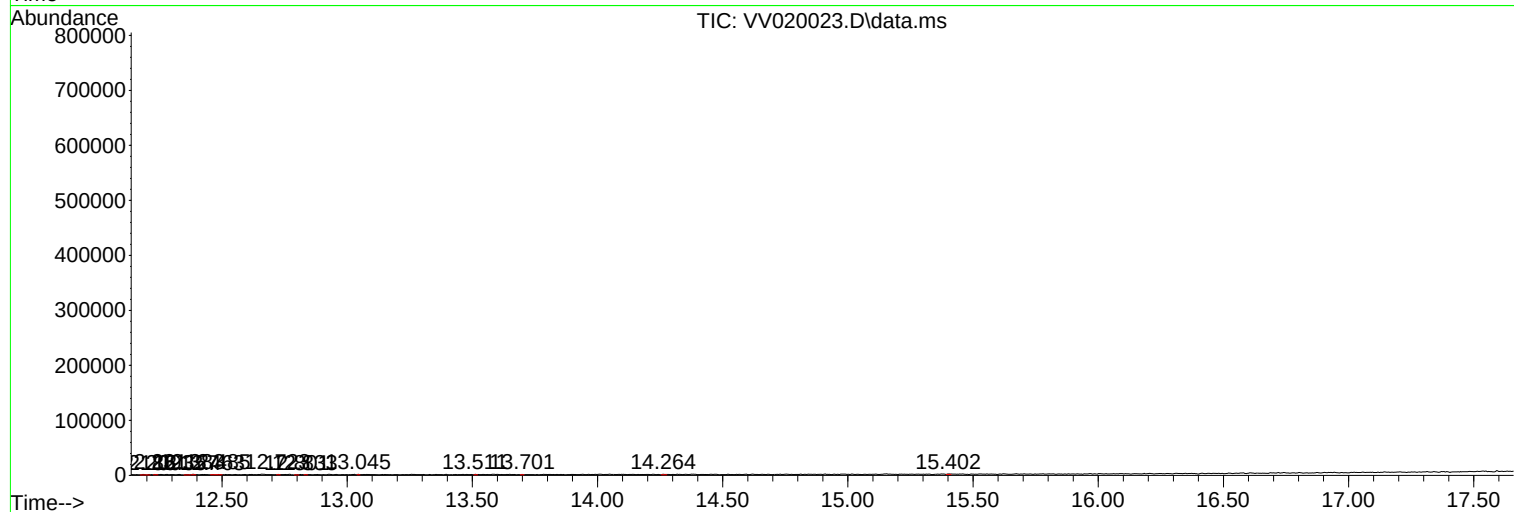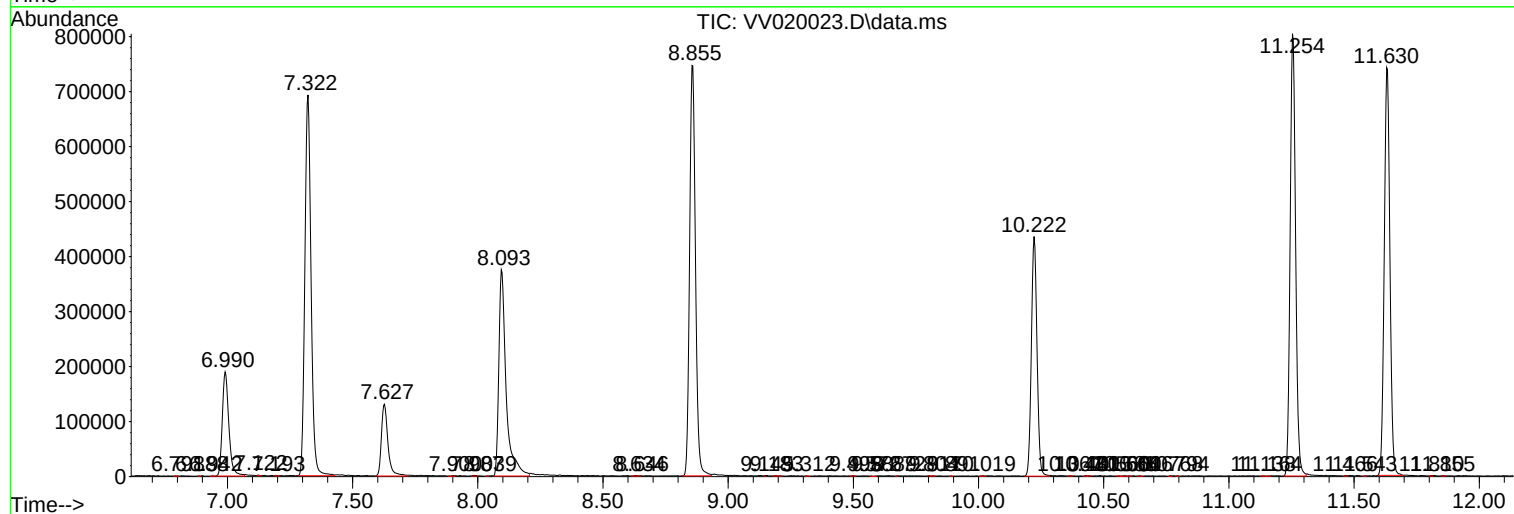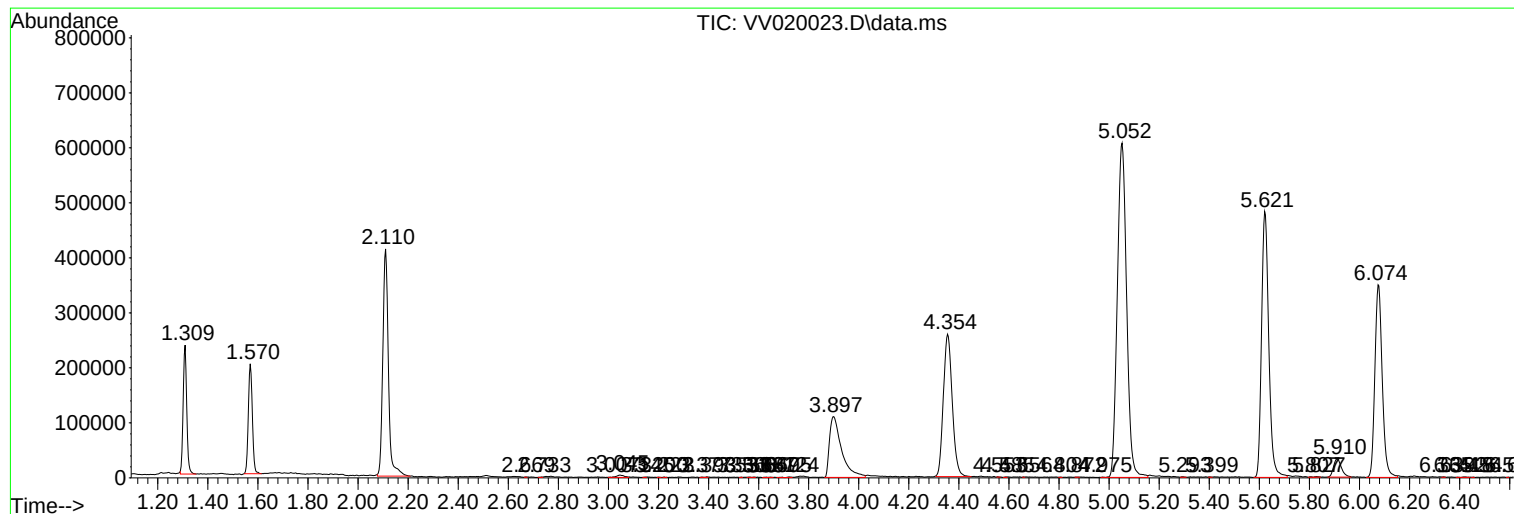

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020023.D
Acq On : 15 Jan 2021 14:11
Operator : SY/MD
Sample : M1147-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020023.D
Acq On : 15 Jan 2021 14:11
Operator : SY/MD
Sample : M1147-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Y6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
