

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020028.D
 Acq On : 15 Jan 2021 16:46
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M

Title : VOC Analysis

Signal : TIC: VV020028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	81	rVB	203196	203828	13.88%	1.734%
2	1.570	142	149	161	rBV	181987	202168	13.77%	1.720%
3	2.110	307	317	345	rVB	373571	570996	38.88%	4.857%
4	2.341	386	389	390	rBV3	976	623	0.04%	0.005%
5	2.685	493	496	498	rBV2	642	429	0.03%	0.004%
6	2.746	513	515	518	rBV3	991	664	0.05%	0.006%
7	2.856	546	549	554	rBV4	686	517	0.04%	0.004%
8	2.894	557	561	565	rBV4	793	697	0.05%	0.006%
9	2.991	589	591	595	rVB5	991	667	0.05%	0.006%
10	3.045	595	608	622	rBV10	3944	9980	0.68%	0.085%
11	3.116	628	630	633	rBV3	810	505	0.03%	0.004%
12	3.164	643	645	649	rBV4	512	344	0.02%	0.003%
13	3.216	657	661	662	rBV	833	491	0.03%	0.004%
14	3.229	663	665	667	rVB2	719	325	0.02%	0.003%
15	3.270	674	678	681	rBV3	684	546	0.04%	0.005%
16	3.393	712	716	719	rBV3	659	484	0.03%	0.004%
17	3.479	736	743	747	rBV3	884	794	0.05%	0.007%
18	3.499	747	749	752	rBV2	642	323	0.02%	0.003%
19	3.531	757	759	762	rBV4	655	406	0.03%	0.003%
20	3.595	778	779	783	rBV3	551	354	0.02%	0.003%
21	3.614	783	785	790	rVB4	782	487	0.03%	0.004%
22	3.647	792	795	798	rBV2	481	357	0.02%	0.003%
23	3.669	798	802	805	rVV3	708	496	0.03%	0.004%
24	3.733	819	822	824	rBV3	551	342	0.02%	0.003%
25	3.759	824	830	831	rBV6	925	795	0.05%	0.007%
26	3.852	852	859	862	rBV3	1024	809	0.06%	0.007%
27	3.897	862	873	900	rBV	107969	330895	22.53%	2.814%
28	4.293	994	996	998	rBV2	750	405	0.03%	0.003%
29	4.354	999	1015	1037	rVV	247459	607861	41.39%	5.170%
30	4.637	1099	1103	1107	rBV4	767	681	0.05%	0.006%
31	4.698	1120	1122	1124	rBV3	775	354	0.02%	0.003%
32	4.730	1129	1132	1133	rBV	636	336	0.02%	0.003%
33	4.923	1189	1192	1195	rVB2	663	399	0.03%	0.003%
34	5.052	1211	1232	1259	rBV2	568308	1468571	100.00%	12.491%
35	5.470	1358	1362	1366	rVB5	1031	864	0.06%	0.007%
36	5.495	1366	1370	1373	rBV2	1244	957	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020028.D
 Acq On : 15 Jan 2021 16:46
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

37	5.540	1381	1384	1389	rBV5	863	692	0.05%	0.006%
38	5.621	1396	1409	1437	rBV	490411	974507	66.36%	8.289%
39	5.910	1488	1499	1520	rBV3	28576	61106	4.16%	0.520%
40	6.013	1526	1531	1533	rBV4	880	734	0.05%	0.006%
41	6.074	1536	1550	1570	rBV	333713	679346	46.26%	5.778%
42	6.312	1621	1624	1629	rBV7	763	630	0.04%	0.005%
43	6.335	1629	1631	1634	rVB2	786	377	0.03%	0.003%
44	6.479	1674	1676	1680	rVB4	1091	684	0.05%	0.006%
45	6.547	1694	1697	1700	rBV3	525	326	0.02%	0.003%
46	6.769	1764	1766	1773	rBV6	773	689	0.05%	0.006%
47	6.926	1810	1815	1817	rBV4	526	406	0.03%	0.003%
48	6.991	1822	1835	1852	rBV	174984	316018	21.52%	2.688%
49	7.322	1926	1938	1963	rBV	632319	1097930	74.76%	9.338%
50	7.627	2022	2033	2050	rBV	119633	213807	14.56%	1.819%
51	7.962	2132	2137	2139	rBV5	1023	743	0.05%	0.006%
52	8.093	2168	2178	2208	rBV2	360170	723425	49.26%	6.153%
53	8.778	2389	2391	2394	rVB4	565	325	0.02%	0.003%
54	8.807	2397	2400	2403	rBV5	727	552	0.04%	0.005%
55	8.859	2403	2416	2441	rBV	748951	1225646	83.46%	10.425%
56	9.254	2535	2539	2546	rBV7	1013	1470	0.10%	0.013%
57	9.392	2577	2582	2584	rBV5	637	670	0.05%	0.006%
58	9.582	2635	2641	2645	rBV4	539	752	0.05%	0.006%
59	9.695	2673	2676	2678	rBV2	608	313	0.02%	0.003%
60	9.756	2690	2695	2697	rBV3	1019	695	0.05%	0.006%
61	9.788	2702	2705	2710	rVB3	854	589	0.04%	0.005%
62	9.820	2710	2715	2718	rBV4	697	776	0.05%	0.007%
63	9.916	2741	2745	2746	rBV	503	335	0.02%	0.003%
64	9.942	2750	2753	2758	rBV3	694	688	0.05%	0.006%
65	9.984	2764	2766	2768	rBV2	597	369	0.03%	0.003%
66	10.055	2786	2788	2792	rBV4	548	317	0.02%	0.003%
67	10.148	2813	2817	2821	rBV3	401	396	0.03%	0.003%
68	10.222	2826	2840	2858	rBV	430502	676205	46.05%	5.751%
69	10.389	2888	2892	2894	rBV4	549	314	0.02%	0.003%
70	10.428	2901	2904	2905	rBV	624	331	0.02%	0.003%
71	10.508	2925	2929	2931	rBV2	650	554	0.04%	0.005%
72	10.714	2988	2993	2996	rBV4	664	591	0.04%	0.005%
73	10.756	3003	3006	3009	rBV	526	503	0.03%	0.004%
74	10.810	3022	3023	3030	rVB6	500	451	0.03%	0.004%
75	10.933	3059	3061	3064	rBV2	749	510	0.03%	0.004%
76	10.997	3078	3081	3084	rBV2	501	428	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
 Data File : VV020028.D
 Acq On : 15 Jan 2021 16:46
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
 Title : VOC Analysis

77	11.074	3101	3105	3106	rBV3	614	349	0.02%	0.003%
78	11.161	3127	3132	3134	rBV4	826	685	0.05%	0.006%
79	11.254	3150	3161	3181	rBV	803231	1237273	84.25%	10.524%
80	11.502	3235	3238	3241	rVB3	991	581	0.04%	0.005%
81	11.579	3261	3262	3264	rBV3	764	379	0.03%	0.003%
82	11.630	3267	3278	3299	rVV	703589	1114229	75.87%	9.477%
83	11.833	3339	3341	3346	rVB4	619	404	0.03%	0.003%
84	12.141	3435	3437	3441	rVB3	632	411	0.03%	0.003%
85	12.309	3484	3489	3494	rVB5	1075	1051	0.07%	0.009%
86	12.334	3494	3497	3500	rBV4	691	616	0.04%	0.005%
87	12.418	3520	3523	3525	rBV2	576	383	0.03%	0.003%
88	12.608	3579	3582	3584	rBV3	978	528	0.04%	0.004%
89	12.637	3587	3591	3592	rBV3	629	344	0.02%	0.003%
90	12.694	3606	3609	3612	rBV4	607	459	0.03%	0.004%
91	12.826	3647	3650	3653	rBV4	563	428	0.03%	0.004%
92	12.900	3670	3673	3678	rBV3	901	680	0.05%	0.006%
93	13.000	3701	3704	3705	rBV3	539	322	0.02%	0.003%
94	13.039	3714	3716	3719	rBV3	509	409	0.03%	0.003%
95	13.106	3733	3737	3739	rBV4	655	455	0.03%	0.004%
96	13.383	3820	3823	3826	rBV4	674	504	0.03%	0.004%
97	13.447	3840	3843	3845	rBV2	647	418	0.03%	0.004%
98	13.498	3857	3859	3862	rBV3	553	368	0.03%	0.003%
99	14.193	4073	4075	4079	rVB	697	401	0.03%	0.003%
100	14.321	4112	4115	4118	rBV4	764	606	0.04%	0.005%




Sum of corrected areas: 11757233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020028.D
Acq On : 15 Jan 2021 16:46
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

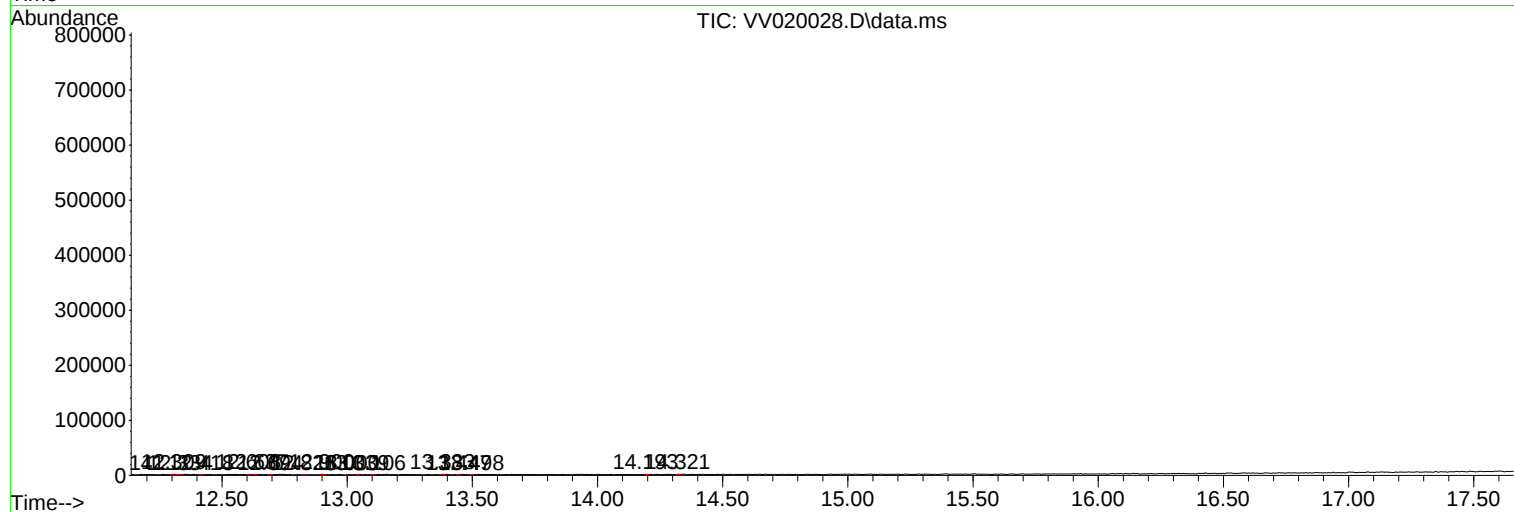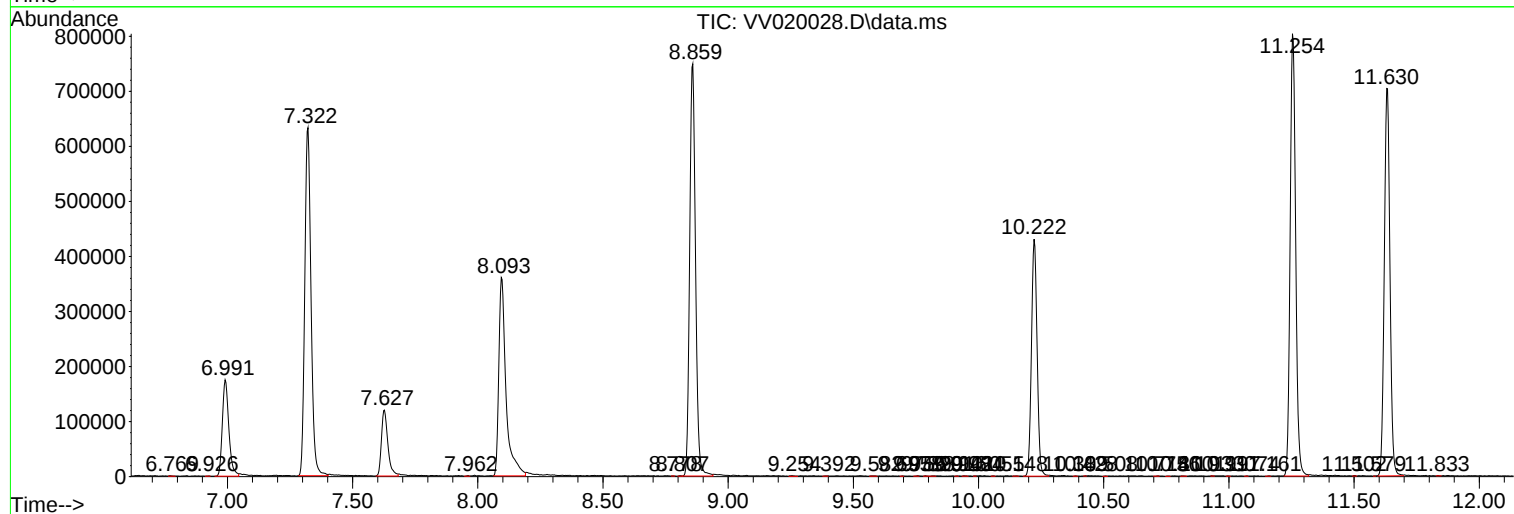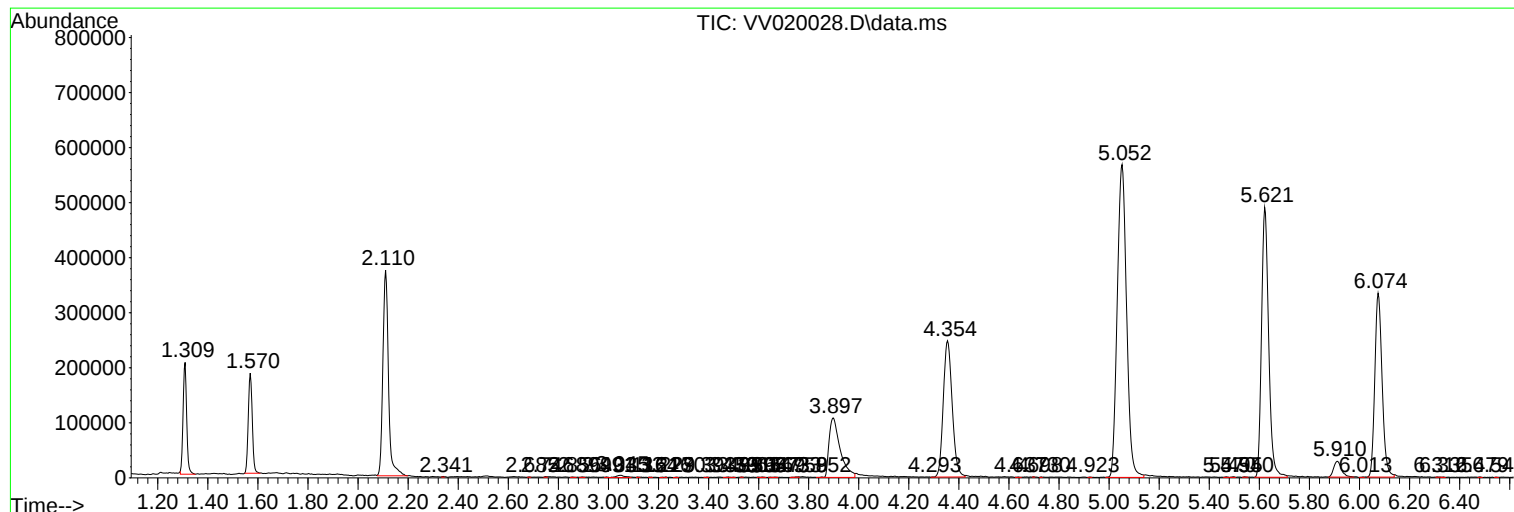

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020028.D
Acq On : 15 Jan 2021 16:46
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011521\
Data File : VV020028.D
Acq On : 15 Jan 2021 16:46
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM011121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
